

REPORT ITU-R BS.2037

Evaluating fields from terrestrial broadcasting transmitting systems operating in any frequency band for assessing exposure to non-ionizing radiation

(Question ITU-R 50/6)

(2004)

TABLE OF CONTENTS

	Page
1 Introduction	3
2 Characteristics of electromagnetic fields.....	3
2.1 General field characteristics	3
2.1.1 Field components.....	3
2.1.2 Far field.....	4
2.1.3 Near field	6
2.1.4 Polarization.....	7
2.1.5 Modulation.....	7
2.1.6 Interference patterns	13
2.2 Field-strength levels near broadcasting antennas	13
2.2.1 LF/MF bands (150-1 605kHz)	13
2.2.2 HF bands (3-30 MHz).....	13
2.2.3 VHF/UHF bands.....	14
2.2.4 SHF (3-30 GHz), 0.1-1 m).....	14
2.3 Mixed frequency field.....	16
2.4 EMF inside buildings.....	17
3 Calculation.....	17
3.1 Procedures.....	17
3.1.1 Closed solutions.....	17
3.1.2 Numerical procedures	18

	Page	
4	Measurements.....	21
4.1	Procedures.....	21
4.1.1	LF/MF bands	21
4.1.2	HF bands.....	21
4.1.3	VHF/UHF bands.....	21
4.1.4	SHF bands.....	22
4.2	Instruments	22
4.2.1	Introduction.....	22
4.2.2	Characteristics of the measurement instruments for electric and magnetic field	23
4.2.3	Narrow-band instrument types and specifications.....	24
4.3	Comparison between predictions and measurements.....	25
5	Precautions at transmitting stations and their vicinity.....	25
5.1	Precautions to control the direct health effects of RF radiation	25
5.1.1	Employee (occupational) precautionary measures	26
5.1.2	Precautionary measures in relation to the general public	27
5.2	Precautions to control the indirect RF radiation hazards.....	28
	Appendix 1 – Examples of calculated field strengths near broadcasting antennas	29
	Appendix 2 – Comparison between predictions and measurements.....	42
	Appendix 3 – Limits and levels	63
	Appendix 4 – Additional evaluation methods.....	72
	Appendix 5 – Electromedical devices.....	77
	Appendix 6 – References	78

1 Introduction

For many years the subject of the effects of electromagnetic radiation has been considered and attempts have been made to quantify particular limits that could be used to protect humans from undesirable effects. Studies in many countries by differing agencies have resulted in various administrative regulations. It is noteworthy and understandable that no single standard has emerged from all the efforts in this regard.

This Report is intended to provide a single basis for the derivation and estimation of the values of electromagnetic radiation from a broadcast station that occur at particular distances from the transmitter site. Using such information, responsible agencies can then develop appropriate standards that may be used to protect humans from undesirable exposure to harmful radiation. The actual values to be applied in any regulation will naturally depend on decisions reached by responsible health agencies, domestic and worldwide.

It is noted that this ITU-R Report and ITU-T Recommendations cover similar material, but with an emphasis on different aspects of the same general subject. For example, ITU-T Recommendations K.51 (Guidance on complying with circuits for human response to electromagnetic fields) and K.61 (Guidance to measurement and numerical prediction of electromagnetic fields for compliance with human limits for telecommunication installations) provide guidance on compliance with exposure limits for telecommunication systems. Appropriate reference information is included in Appendix 6.

2 Characteristics of electromagnetic fields

2.1 General field characteristics

This section gives an overview of the special characteristics of electromagnetic (EM) fields that are relevant to this Report, especially the distinction between the near field and the far field. Simple equations are derived for calculating the power density and the field strength in the far field, and the section concludes by defining the terms polarization and interference patterns.

2.1.1 Field components

The EM field radiated from an antenna comprises various electric and magnetic field components, which attenuate with distance, r , from the source. The main components are:

- the far field (Fraunhofer), also called the radiation field, in which the magnitude of the fields diminishes at the rate of $1/r$;
- the radiating near field (Fresnel), also called the inductive field. The field structure of the inductive field is highly dependent on the shape, size and type of the antenna although various criteria have been established and are commonly used to specify this behaviour;
- the reactive near field (Rayleigh), also called quasi-static field, which diminishes at the rate of $1/r^3$.

As the inductive and quasi-static components attenuate rapidly with increasing distance from the radiation source, they are only of significance very close to the transmitting antenna – in the so-called *near-field* region.

The radiation field, on the other hand, is the dominant element in the so-called far-field region. It is the radiation field, which effectively carries a radio or television signal from the transmitter to a distant receiver.

2.1.2 Far field

In the far-field region, an electromagnetic field is predominantly plane wave in character. This means that the electric and magnetic fields are in phase, and that their amplitudes have a constant ratio. Furthermore, the electric fields and magnetic fields are situated at right angles to one another, lying in a plane, which is perpendicular to the direction of propagation.

It is often taken that far-field conditions apply at distances greater than $2D^2/\lambda$ where D is the maximum linear dimension of the antenna.

However, care must be exercised when applying this condition to broadcast antennas for the following reasons:

- it is derived from considerations relating to planar antennas;
- it is assumed that D is large compared with λ .

Where the above conditions are not met, a distance greater than 10λ should be used for far field.

2.1.2.1 Power density

The power density vector, the Poynting vector \mathbf{S} , of an electromagnetic field is given by the vector product of the electric, \mathbf{E} , and magnetic, \mathbf{H} , field components:

$$\mathbf{S} = \mathbf{E} \times \mathbf{H} \quad (1)$$

In the far field, in ideal conditions where no influence of the ground or obstacles is significant, this expression can be simplified because the electric and magnetic fields, and the direction of propagation, are all mutually orthogonal. Furthermore, the ratio of the electric, E , and magnetic, H , field strength amplitudes is a constant, Z_0 , which is known as the characteristic impedance of free space¹ and is about 377Ω (or $120\pi \Omega$).

Thus, in the far field, the power density, S , in free space is given by the following non-vector equation:

$$S = E^2/Z_0 = H^2 Z_0 \quad (2)$$

¹ Generally, the characteristic impedance of a medium is given by $z = \sqrt{(\mu/\epsilon)}$ where μ is the magnetic permeability ($= 1.2566 \times 10^{-6}$ F/m in free space), and ϵ is the permittivity ($= 8.85418 \times 10^{-12}$ H/m in free space).

The power density – at any given distance in any direction – can be calculated in the far field using the following equation:

$$S = P G_i / (4\pi r^2) \quad (3)$$

where:

S : power density (W/m²) in a given direction

P : power (W) supplied to the radiation source, assuming a lossless system

G_i : gain factor of the radiation source in the relevant direction, relative to an isotropic radiator

r : distance (m) from the radiation source.

The product PG_i in equation (3) is known as the e.i.r.p. which represents the power that a fictitious isotropic radiator would have to emit in order to produce the same field intensity at the receiving point.

For power densities in other directions the antenna pattern must be taken into account.

In order to use equation (3) with an antenna design whose gain G_a is quoted relative to a reference antenna of isotropic gain G_r , such as a half-wave dipole or a short monopole, the gain factor G_i must be replaced by the product of $G_r \cdot G_a$, as in equation (4). The relevant factor G_r is given in Table 1.

$$S = P G_r G_a / (4\pi r^2) \quad (4)$$

TABLE 1

Isotropic gain factors for different types of reference antenna

Reference antenna type	Isotropic gain factor G_r	Typical applications where reference antenna type is relevant
Isotropic radiator	1.0	Radar, satellite and terrestrial radio link system
Half-wave dipole	1.64	Television, VHF and sometimes HF broadcasting
Short monopole	3.0	LF, MF and sometimes HF broadcasting

Thus, when the gain of the antenna G_d ($G_a = G_d$) is expressed relative to that of a half-wave dipole:

$$S = 1.64 P G_d / (4\pi r^2) \quad (5)$$

where:

G_d : gain of the antenna relative to a half-wave dipole.

Similarly, when the gain of the antenna $G_a = G_m$ is expressed relative to that of a short monopole:

$$S = 3.0 P G_m / (4\pi r^2) \quad (6)$$

where:

G_m : gain of the antenna relative to a short monopole.

2.1.2.2 Field strength

Equations (2)-(10) assume plane wave (far-field) conditions and are not applicable to near-field calculations.

If equation (2) is inserted into equation (3) to eliminate S , and a factor C is introduced to take account of the directional characteristic of the radiation source, then equation (7) is obtained for the electric field strength in the far field of a radiation source:

$$E = \sqrt{\frac{Z_0}{4\pi}} \frac{\sqrt{PG_i}}{r} \quad C = \frac{C}{r} \sqrt{30PG_i} \quad (7)$$

where:

E : electric field strength (V/m)

$Z_0 = 377 \Omega$, the characteristic impedance of free space

P : power fed to the radiation source (W), assuming a lossless system

C : factor ($0 \leq C \leq 1$), which takes account of the directional characteristic of the radiation source (in the main direction of radiation, $C = 1$).

If the gain of the antenna is expressed relative to a half-wave dipole or a short monopole, rather than relative to an isotropic radiator, then the factors G_d or G_m , respectively, should be used in place of G_i , as shown in equations (8) and (9).

$$E = \sqrt{\frac{Z_0}{4\pi}} \frac{\sqrt{1.64PG_d}}{r} \quad C = \frac{C}{r} \sqrt{49.2PG_d} \quad (8)$$

$$E = \sqrt{\frac{Z_0}{4\pi}} \frac{\sqrt{3PG_m}}{r} \quad C = \frac{C}{r} \sqrt{90PG_m} \quad (9)$$

In order to calculate the magnetic field strength in the far field of a radiation source, equation (10) is used:

$$H = E/Z_0 \quad (10)$$

where:

E : electric field strength (V/m)

H : magnetic field strength (A/m)

$Z_0 = 377 \Omega$ (120π), the characteristic impedance of free space.

2.1.3 Near field

The field structure in the near-field region is more complex than that described above for the far field. In the near field, there is an arbitrary phase and amplitude relationship between the electric and magnetic field strength vectors, and the field strengths vary considerably from point to point. Consequently, when determining the nature of the near field, both the phase and the amplitude of both the electric and magnetic fields must be calculated or measured. In practice, however, this may prove very difficult to accomplish.

2.1.3.1 Power density and field strength

It is not easy to determine the Poynting vector in the near field because of the arbitrary phase and amplitude relationship mentioned above. The E and H amplitudes, together with their phase relationship, must be measured or calculated separately at each point, making the task particularly complex and time-consuming.

Using analytical formulas, an estimation of the field strength in the near field is only feasible for simple ideal radiators such as the elementary dipole. In the case of more complex antenna systems, other mathematical techniques must be used to estimate field strength levels in the near-field region. These other techniques allow relatively precise estimations of the field strength, the power density and other relevant characteristics of the field, even in the complex near-field region.

Measurement in the near field is even more difficult as no reference calibration method exists. The International Electrotechnical Commission is currently working on the issue of a measurement standard for high frequency (9 kHz to 300 GHz) electromagnetic fields particularly in the near field [1]. In addition, EN 61566 (Measurements of exposure to Radiofrequency electromagnetic field strength in the frequency range 1 kHz-1 GHz – sub-clause 6.1.4) gives more information on this topic.

2.1.4 Polarization

Polarization is defined as the direction of the electric field vector, referenced to the direction of propagation of the wave front.

In broadcasting, different types of polarization are used. The main types are vertical and horizontal (with respect to a wave front which is travelling parallel to the surface of the Earth) although other types of polarization are used such as slant and elliptical.

2.1.5 Modulation

Modulation is a very special characteristic of the emission from a broadcasting transmitter. As certain effects of EM radiation are sensitive to the type of modulation used, it follows that the presence of modulation must be taken into consideration when making safety assessments. Modulation must also be taken into consideration when carrying out measurements or calculations to determine whether or not the limits are being exceeded.

The modulation often results in a signal varying in both amplitude and frequency. For this reason temporal averaging is usually required in determining the values to be used in measurement and calculation. This requirement is also acknowledged in relevant Standards.

2.1.5.1 Characteristics of radio emission

The Radio Regulations (RR) classify the emissions from radio transmitters according to the required bandwidths, and the basic and optional characteristics of the transmission. The complete classification consists of nine characters as follows:

- Characters 1-4 describe the bandwidth, using three digits and one letter;
- Characters 5-7 describe the basic characteristics, using two letters and one digit;
- Characters 8-9 describe any optional characteristics, using two letters.

Only the three basic characteristics are relevant to the consideration of RF safety considerations. These are:

- the type of modulation of the main carrier Character 5
- the nature of the signal(s) which modulate(s) the main carrier Character 6
- the type of information to be transmitted Character 7

Table 2, which is based on information given in the RR, lists the various characters which are used to classify the three basic characteristics of a radio emission. For sound and television broadcasts, the relevant characters are as follows:

- AM radio (LF, MF and HF double sideband) A3E
- AM radio (HF single sideband, reduced/variable carrier) R3E
- AM radio (HF single sideband, suppressed carrier) J3E
- Television pictures C3F
- Television sound F3E or A3E
- FM radio F3E or F9E
- DVB G7F
- DAB G7E

TABLE 2

Characters used to define the class of emission, based on information given in the RR

Character 5 Type of modulation of the main carrier		Character 6 Nature of the signal(s) modulating the main carrier		Character 7 Type of information to be transmitted	
N	Unmodulated	0	No modulating signal	N	No information transmitted
A	Amplitude modulation: double-sideband	1	Single channel containing: quantized or digital information <i>not</i> using a modulating sub-carrier	A	Telegraphy for aural reception
H	Amplitude modulation: single-sideband, full carrier	2	Single channel containing: quantized or digital information using a modulating sub-carrier	B	Telegraphy for automatic reception
R	Amplitude modulation: single-sideband, reduced or variable-level carrier	3	Single channel containing: analogue information	C	Facsimile
J	Amplitude modulation: single-sideband, suppressed carrier	7	Two or more channels containing: quantized or digital information	D	Data transmission, telemetry and telecommand

TABLE 2 (*end*)

Character 5 Type of modulation of the main carrier		Character 6 Nature of the signal(s) modulating the main carrier		Character 7 Type of information to be transmitted	
B	Amplitude modulation: independent sidebands	8	Two or more channels containing: analogue information	E	Telephony including sound broadcasting
C	Amplitude modulation: vestigial sideband	9	Two or more channels containing: a mix of analogue and digital channels	F	Television (video)
F	Angle modulation: frequency (i.e. FM)	X	Cases not otherwise covered	W	Combination of the above
G	Angle modulation: phase			X	Cases not otherwise covered
D	Mixture of amplitude and angle modulation (simultaneously or sequentially)				
P	Sequence of pulses: unmodulated				
K	Sequence of pulses: modulated in amplitude				
L	Sequence of pulses: modulated in width/duration				
M	Sequence of pulses: modulated in position/phase				
Q	Sequence of pulses: angle-modulation of the carrier during the period of the pulse				
V	Sequence of pulses: combination of K, L, M and Q, or produced by other means				
W	Cases not covered above: Carrier modulated by two or more modes (amplitude, angle, pulse)				
X	Cases not otherwise covered				

2.1.5.2 Expressing transmitter power and field strength in terms of modulation type

Information about the transmitter power supplied to the antenna and the type of modulation can be obtained from the transmission authority, which is responsible for operating the equipment at a particular site. It is important to know whether the transmitter power is expressed in terms of the carrier power, P_c , the mean power, P_m , or the peak power, P_p , so that the measured or calculated values can be compared accurately with the derived levels.

TABLE 3a (end)

Class of emission (basic characteristics) (1), (2)	Known power type								
	Carrier power, P_c			Mean power, P_m			Peak power, P_p		
	Factor for the determination of:			Factor for the determination of:			Factor for the determination of:		
	P_c	P_m	P_p	P_c	P_m	P_p	P_c	P_m	P_p
C*F ⁽⁴⁾ Negative modulation Positive modulation	–	–	–	–	1	1.85	–	0.54	1
F*... ⁽⁵⁾	1	1	1	1	1	1	1	1	1
H*A H*B H*E	1	2	4	0.5	1	2	0.25	0.5	1
J*B ⁽³⁾ J*C ⁽³⁾ J*E ⁽³⁾	–	–	–	0	1	1	0	1	1
K*A K*E	1	1.5	4/d	0.67	1	2.67/d	0.25d	0.38d	1
L*A L*E M*A H*E P*N	1	1	1/d	1	1	1/d	d	d	1
R*B ⁽³⁾ R*C ⁽³⁾ R*E ⁽³⁾	–	–	–	–	1	1	–	1	1
G7E	1	1	1	1	1	1	1	1	1
G7F	1	1	1	1	1	1	1	1	1

(1) See Table 2 for further information on the 3-symbol code, which is used to describe the three basic characteristics of a transmission type.

(2) An * indicates that the 2nd characteristic (i.e. the nature of the modulating signal) is not relevant to the consideration of hazards.

(3) It is assumed that the carrier is almost totally suppressed and that, in the case of modulation with a tone, the peak power of the transmitter can be reached in an SSB.

(4) Carrier power, P_c , is not clearly defined.

(5) The 3rd characteristic is not relevant to the consideration of hazards.

d = pulse duty factor.

These factors are given for DAB and DVB when measuring over the whole channel power (generally 1.5 MHz for DAB and 8 MHz for DVB)

TABLE 3b

**Relationship between carrier, average, peak and maximum instantaneous power,
for different classes of emission (typical case modulation)**

Class of emission (basic characteristics)	Known power type								
	Carrier power, P_c			Mean power, P_m			Peak power P_p		
	Factor for the determination of:			Factor for the determination of:			Factor for the determination of:		
	P_c	P_m	P_p	P_c	P_m	P_p	P_c	P_m	P_p
A*C (for $m = 70\%$) A*E (for $m = 70\%$)	1	1.25	4	0.67	1	2.67	0.25	0.38	1
C*F ⁽¹⁾									
Negative modulation	–	–	–	–	1	4.34	–	0.23	1
Positive modulation	–	–	–	–	1	2.7	–	0.37	1
F*...	1	1	1	1	1	1	1	1	1

⁽¹⁾ Carrier power, P_c , is not clearly defined.

Table 3b can also be used to convert field strength values to other notations; note, however, that the square root of the conversion factors given in Table 3b must be used when dealing with field strengths. Thus, in the above example of AM radio, the carrier-only RMS field-strength should be multiplied by $\sqrt{1.5}$ (or $\sqrt{1.25}$) to give the RMS field strength, which includes the modulation components. Conversely, the derived level (including modulation components) should be divided by $\sqrt{1.5}$ (or $\sqrt{1.25}$) to give an equivalent derived level for the carrier only.

The r.m.s. value of the field strength in the far field can be calculated from the known power, using equation (7); the appropriate type of power to use (i.e. P_m , or P_p) is shown in Table 4.

TABLE 4

Relationship between certain field-strength notations and power notations

To calculate	Use power expressed as
The effective value of the equivalent field-strength	Average transmitter power, P_m
The average value of the equivalent field-strength which occurs during a period of peak RF oscillation	Peak power, P_p
Peak (maximum) value of the equivalent field-strength	Peak power, $P_p^{(1)}$

⁽¹⁾ The peak value of the equivalent field strength is determined from the peak power, P_p , using the peak/r.m.s. correction factor. This factor is $2^{1/2}$ for a sinusoidal carrier.

2.1.6 Interference patterns

Both natural and man-made structures can reradiate an electromagnetic field (EMF). The reradiated field adds vectorially to the direct field. This can result in interference patterns, which are comprised of localized maxima and minima of the field strength. The interference pattern is even more complex if there are multiple reradiations of the field.

Interference patterns depend on the frequency of the radiation source. The higher the frequency, the smaller the wavelength and hence the closer, spatially, the maxima and minima. At UHF television frequencies, the local maxima and minima may be separated by only tens of centimetres.

Several overlapping patterns occur in the case of multiple-radiation sources, e.g. if several radio and television channels are radiated from the same site.

2.2 Field-strength levels near broadcasting antennas

In this section, the field-strength levels which are found in the vicinity of typical LF/MF, HF, VHF and UHF broadcasting antennas are discussed.

2.2.1 LF/MF bands (150-1 605 kHz)

At LF and MF, the frequencies are below whole-body resonance frequencies. In the case of direct effects, the limit (also defined as “derived”) levels for both the electric, E , and magnetic, H , field values are relatively high; in many cases, high values are present only very close to the antenna. This is especially true at the lower end of the LF/MF range, and for those standards/guidelines, which have specified higher derived levels. At the upper end of the band, however, the relevant distances may extend to the order of a few hundred metres. It should be realized that this increase in distance is due, in part at least, to the reduction in reference levels at the upper end of the MF band. During transmissions, access to the mast/tower must be avoided, owing to the high field-strengths and the risk of electric shock.

2.2.2 HF bands (3-30 MHz)

Measurements suggest that large areas around a high-power HF transmitting station the EMF will exceed the derived electric field-strength levels, especially near open-wire feeders. At many broadcasting stations, these feeders are now being encased by trunking to reduce the field, but this cannot be done around the antenna arrays themselves. Thus, some parts of the land containing the antenna arrays will have to become “exclusion areas” and maintenance schedules will have to be planned to avoid times when the array is transmitting. This will be difficult on many HF stations where, for programming requirements, the field patterns may change every 15 min. The field-

strength in front of an HF array tends to increase with height above the ground. This is partly because the main beam has an angle of elevation of around 10° to 15° , but mainly results from the boundary conditions at the surface of the ground. Most HF broadcast antennas are horizontally polarized, in which case the electric field-strength at the ground would be zero for an infinitely conducting earth. In practice however, owing to the finite conductivity of the ground, there is a small horizontal component of the electric field.

It is important to realize that the near field of an HF antenna array may extend a considerable distance. This is not only because of the size of the antennas, but also because uneven terrain can result in a very large effective aperture for the array. This results in the field-strength measurements falling below the derived levels at locations close to the array, then rising again with increasing distance from the antennas. However, once the far-field region is entered, the field-strength levels follow the normal pattern of decreasing with increased distance from the antenna array.

2.2.3 VHF/UHF bands

Normally, at high power VHF/UHF sites, the antennas are generally located about 100 m above the ground level, mounted on masts or self-supporting towers. On the ground level, therefore, the field-strengths are relatively low, owing to the distance from the antenna and also to the narrow beamwidth transmitted in the vertical plane.

2.2.4 SHF (3-30 GHz), (0.1-1 m)

This frequency band is used for an enormous number of telecommunication services, such as point-to-point and point-to-multipoint fixed and mobile microwave links, satellite broadcasting, civil and military radars, earth uplink stations, etc.

In the following sub-sections the systems used in broadcasting are treated.

2.2.4.1 Field area definitions


For dish antennas with diameter $D \gg \lambda$ the following definitions are used:

Near-field region – In the near-field, or Fresnel region, of the main beam, the power density can reach a maximum before it begins to decrease with distance. The maximum value of the near field power density on axis depends only on power fed to antenna, the diameter, D , of the antenna, and the efficiency of antenna.

Transition region – The power density in the transition region decreases inversely with distance from the antenna.

Far-field region – The power density in the far-field, or Fraunhofer region, of the antenna pattern decreases inversely as the square of the distance.

The various zones of a parabolic antenna are shown in Fig. 1. The following approach is only valid along the main axis of the antenna.

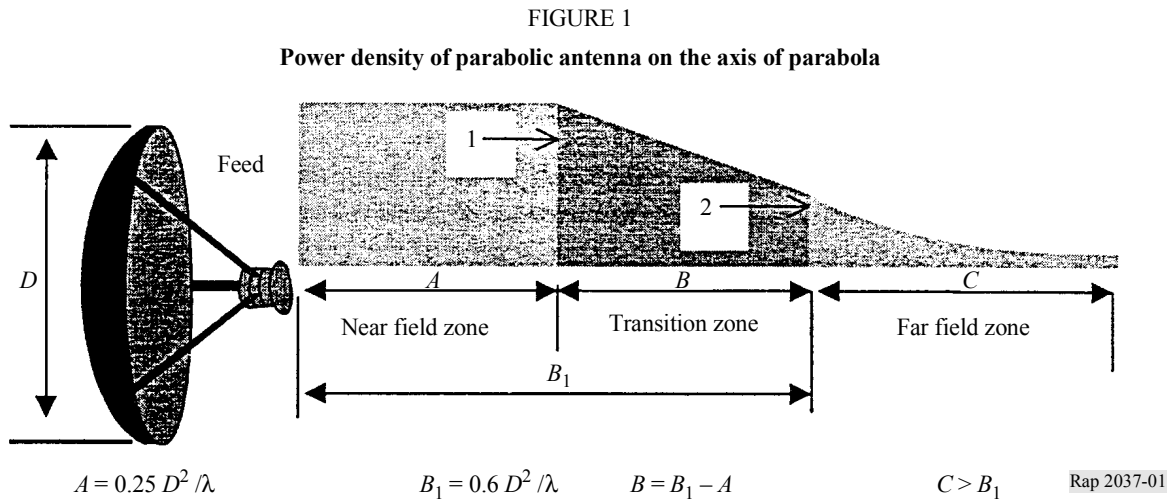

The radiation of a parabolic antenna in the near-field zone occurs along the entire length of the zone in the form of a cylinder with a diameter, D . The maximum of the EMF and its power density are constant throughout the near-field zone.

It is expressed by the equation:

$$S \text{ (W/m}^2\text{)} = \frac{16\eta P}{\pi D^2}$$

where:

- η : efficiency of parabolic antenna (0.55 is used)
- P : power of transmitter (W)
- D : diameter of parabolic antenna (m).

It should be noted that the density, S , is maximal throughout the near-field zone.

From point 1 (beginning of the transition zone) the density S decreases linearly with the distance r to point 2, where the far-field zone begins.

In the far-field zone, S decreases with the square of distance according to the equation:

$$S \text{ (W/m}^2\text{)} = \frac{G P}{4\pi r^2}$$

where:

- G : gain of parabolic antenna with respect to an isotropic source
- r : distance from the parabolic antenna (m).

The density S is maximal on the axis of the parabolic antenna.

2.2.4.2 Fixed and mobile terrestrial microwave links

A typical transmitting-receiving system consists of a transmitter-receiver, a waveguide and a transmitting-receiving parabolic antenna. The transmitter powers are within the range from 0.1 W to 15 W and the parabola sizes within the range from 0.5 m to 4 m, both depending on frequency band used.

The gain of the parabolic antennas used lies within the range of 30 dB to 50 dB.

2.2.4.3 Satellite earth stations

An ideal location for a satellite earth station is in lowland, on flat ground, and valleys far from other objects and industrial zones. In practice, however, such stations are often situated in urban areas, on the roofs of buildings, etc.

Generally, the angle of elevation of the main beam is between 5° and 50°; the antenna size is usually up to 15 m, although there are a few examples of larger dishes.

In the near field, the field strength of the fixed and mobile terrestrial links can exceed the reference levels, especially when higher powers are involved. Therefore direct access of any unauthorized persons should be prevented physically. The reference levels can also be exceeded in the transition zone in addition to the near field.

In particular, satellite earth stations of higher powers can, to a large extent, produce fields which exceed the recommended levels both in the near field and in the transition zones. Since these regions can be quite extended, the location of the satellite earth station should be carefully selected. Since the radiation is emitted at a certain elevation angle, safety mechanisms should be included so as to mechanically prevent any alteration of the elevation angle into the position which would allow radiation to be directed in the space where any people may be present.

2.3 Mixed frequency field

It is very often to have more than one transmitter (using different transmitting frequencies) located at the same transmitter site. In that case it is necessary to consider a total (combined) effect on human exposure to RF energy. On the other side, effect is frequency dependent, and therefore, after calculation of the relevant parameters (S , E , and H), combined effect should be taken into account.

For thermal effect, exposure limits are given in terms of specific absorption rate (SAR) (see Appendix 4), what means that appropriate power-densities should be determined. In the case of the multi-frequency transmitter site, the total power-density is recommended to be the sum of the power-density at each transmitting frequency:

$$S_t = \sum_{i=1}^n S_i \quad (11)$$

where S_i is power density at the frequency f_i ($i = 1, 2, \dots, n$), with the condition that:

$$\sum_{i=1}^n \frac{S_i}{L_i} \leq 1 \quad (12)$$

where L_i is the power-density reference level, at the frequency f_i ($i = 1, 2, \dots, n$).

This is the basic principle, but there are some differences how the principle is applied (see Appendix 4).

2.4 EMF inside buildings

The materials of the building and infrastructure inside the building have very strong influence on the EMF, causing variations of the resulting field, from point to point, even in the same room. Spatial variations in the electromagnetic field are caused by multiple reflections of the incident wave, and therefore, polarization of the resulting field may differ from that of the incident wave.

Metallic object and ducts (lines and tubes), making re-radiation (acting as secondary source), may change intensity of the fields in their vicinity.

All these conditions make assessment of the exposure very difficult. Rather large number of parameters should be taken into consideration when carrying out calculation or measurement.

To have acceptable accuracy in calculation of exposure it is necessary to choose appropriate model for representing the environment.

Accuracy of measurement depends on the size and detection tape of the probe, as well as the location of the person who is doing measurements relative to radiation source and probe.

There are no international standards for calculation and measurement method yet.

The critical issue is not simply the value of the exposure limits themselves, but the way in which calculations and measurement should be carried out and that is the main goal of this Report.

3 Calculation

3.1 Procedures

Analytical and numerical calculation methods can predict the external or internal fields from an electromagnetic radiator. Calculations are useful to estimate the level of the field strengths in a certain exposure situation in order to determine if measurements are needed and what equipment should be used. Calculations can also be a complement to measurements and be used to verify that the results from the measurements are reasonable.

In some situations, for example for complicated near-field exposure conditions when expensive SAR measurement equipment are not available, calculations can replace measurements.

The accuracy and quality of the calculations will depend on the analytical or numerical method used and on the accuracy of the description of the electromagnetic source(s) and physical objects between the radiator and the prediction point that may affect the fields. For SAR calculations, the accuracy of the body model will also affect the quality of the results.

To be able to make a calculation, the source parameters have to be known or estimated.

Example of source parameters are frequency, mean power, peak power, pulse width, pulse length, pulse repetition rate and antenna pattern.

3.1.1 Closed solutions

In the far-field region of a transmitting source, where the EMF are predominantly plane wave in character, analytical expressions can be used to estimate the field strengths. In the main direction of

an antenna, the Friis free space equation can be used to calculate the power density:

$$S = \frac{P G}{4\pi d^2}$$

where:

- S : power density in (W/m²)
- P : mean output power (W)
- G : antenna far-field gain relative to an isotropic radiator
- d : distance from radiator (m).

The relation between power density and electric and magnetic field strengths is given by the following equation:

$$S = \frac{E^2}{\eta} = H^2 \eta$$

where:

- E : electric field strength (V/m) (RMS)
- H : magnetic field strength (A/m) (RMS)
- η : The intrinsic impedance of free space, 377 Ω .

Hence, using the above formulas the fields strengths can be calculated:

$$E = \sqrt{\frac{P G \eta}{4\pi d^2}} = \frac{5.5\sqrt{P G}}{d}$$

$$H = \sqrt{\frac{P G}{4\pi d^2 \eta}} = \frac{\sqrt{P G}}{68.8d}$$

These relations are only valid in the far-field region of the radiating source, i.e. when $d > 2D^2/\lambda$, where D is the largest dimension of the radiating structure and λ is the wavelength. Field strength attenuation or enhancement due to reflection, material transmission, and diffraction is not taken into account. Using the relations above in the near-field region, or in directions other than the main direction, will generally give too large values unless a near field correction factor or a radiation pattern factor is introduced.

3.1.2 Numerical procedures

Analytical procedures can only be used to calculate the electromagnetic properties for a few special cases and geometries. To solve general problems, numerical techniques have to be applied. The most common numerical procedures to calculate the EMF from a transmitting source or the internal fields and the specific absorption rate in biological bodies, are listed below. Which of the numerical techniques that is most appropriate for a certain problem, depends on the frequency range considered, the geometrical structures to be modelled, and the type exposure situation (near-field or far-field).

Some usual numerical modelling methods are given below:

- physical optics (PO)
- physical theory of diffraction (PTD)
- geometrical optics (GO)
- geometrical theory of diffraction (GTD)
- uniform theory of diffraction (UTD)
- method of equivalent currents (MEC)
- method of moments (MOM)
- multiple multipole method (MMP)
- finite-difference time-domain method (FDTD)
- finite element method (FEM)
- impedance method.

An assessment must be carried out, for each application, to establish which one of the above methods is the most suitable for solving a given problem.

Each of these procedures enables the amplitude and phase of the following EMF field quantities to be determined, at every point in space, where the radiating and scattering elements may be either ideal conductors or dielectric bodies:

- electric field-strength;
- magnetic field-strength;
- power-density;
- current;
- voltage;
- impedance.

Method of moments (MOM)

The method of moments is often used in the design of broadcast antenna systems (transmitter output power, antenna gain, etc.) and in calculating their resultant electromagnetic fields. It enables calculations to be made at both the transmitting and receiving ends, as well as in the near and far fields of the antenna.

Technical structures with up to three dimensions can be modelled, taking into account their material parameters (complex dielectric constant) as well as that of the ground. The modelling works with wires that are thin with respect to the wavelength and, in principle, is able to represent surfaces too. The limitation of this method lies in the fact that the modelling of extended and complicated structures may become too time – and memory – consuming for the computer.

The method of moments is a technique which has been extensively used to solve electromagnetic problems and to make SAR calculations in block models of biological bodies. In MOM, the electric fields inside a biological body is calculated by means of a Green's function solution of Maxwell's integral equations.

Fast Fourier transform/Conjugate gradient method (FFT/CG)

The FFT/CG method is a further development of the method of moments. Iterative algorithms based on FFT and the gradient procedure are used to solve linear equations derived from the method of moments.

Finite-difference time-domain method (FDTD)

FDTD is a numerical method to solve Maxwell's differential curl equations in the time domain. It can be used to calculate internal and external EMF and SAR distribution in biological bodies for both near-field or far-field exposures. In FDTD, both time and space are discretized, and a biological body is modelled by assigning the permittivity and conductivity values to the space cells it occupies. The computer memory required is proportional to the number of space cells. FDTD is considered the most promising SAR calculation method, but for accurate calculations very powerful computers are needed.

Multiple multipole method (MMP)

MMP is based on analytical solutions to field equations which have a multipole at one point in space, and is used in conjunction with the generalized multipole technique (GMP). The MMP procedure is especially suitable for the simulation of so-called "lossy scattering" bodies, which are near to radiation sources, i.e. within the immediate near-field.

Impedance method

The impedance method has been successfully used to solve dosimetric problems where quasistatic approximations can be made. For calculations of SAR in human bodies, this method has proven to be very effective at frequencies up to 40 MHz. In the impedance method, the biological body is modelled by a three-dimensional network of complex impedances.

3.1.2.1 Field strength calculations

Most of the methods listed above can be used to calculate field strength levels from electromagnetic radiators. The accuracy of the results depends very much on how well the radiator (for example antenna) is modelled. If objects near the radiator, between the radiator and the prediction point, or close to the point of field strength prediction may affect the field strength levels significantly, such objects should also be modelled.

3.1.2.2 Specific absorption rate calculations

Due to the difficulty to measure the whole-body averaged or local peak SAR in many exposure situations, numerical calculations, several of the numerical techniques mentioned above can be used for estimation of the specific absorption rate distribution in a biological body exposed to either near-field or far-field electromagnetic radiation, for example the FDTD, MOM, and the MMP.

Which of these methods that is most appropriate for a particular problem, depends e.g. on the frequency, the exposure conditions, the size of the exposed object, the required accuracy, and the maximum tolerable calculation time. Each method requires experience in biophysics and numerical analysis.

To use any of these models, a three-dimensional geometric numerical model of the exposed body, or part of the body, is required. The electrical properties at the exposure frequency should be known for the different parts of the body. Depending on the required accuracy, models with different complexity may be used. In some situations, simple shapes like spheres and cylinders are appropriate to model the body. The dielectric properties of human tissues are given in the literature. Using magnetic resonance (MR) images of a human body, very complex and accurate numerical body models can be developed. MR models with several different tissue types and a spatial resolution of less than a few millimetres have been used for FDTD calculations of the SAR distribution in humans exposed to electromagnetic fields from handheld radio transmitters.

4 Measurements

4.1 Procedures

It should be noted that, generally speaking, methods of measurement are very important. For near field strength measurements it is, even more, important. For lower frequency bands method of measurement is very sensitive and complex matter, having in mind that, usually, the distance of test point (from source of radiation) is much smaller than wavelength. For that reason, frequency range 10 kHz-30 GHz is divided to four main broadcasting bands: LF/MF, HF, VHF/UHF and SHF bands.

4.1.1 LF/MF bands

In order to verify the theoretical results, field strength measurements in the near zone shall be effectuated by using special instruments (field strength meters) with three orthogonal positioned short dipoles. It is recommended to not use any instrument requesting power supply cable.

To prevent disturbing influence of the person performing a measurement, measuring instrument shall be attached to insulated rod. The distance between instrument and operator should be determined by taking into account that there are no any changes on the instrument scale caused by any movement of the operator. That distance is dependent of the frequency of measured signal.

Performing this kind of measurements it is necessary to take into account possible influence of the all objects in the vicinity, and, particularly those, which could create reradiation effects.

When the purpose of a measurement is to verify results obtained by the theoretical computation, test points should be selected along a radial direction and at height between 1 and 2 m.

More detailed explanation is given in Recommendation ITU-R BS.1386.

4.1.2 HF bands

Detailed explanation is given in Recommendation ITU-R BS.705.

4.1.3 VHF/UHF bands

Detailed explanation is given in Recommendation ITU-R BS.1195.

4.1.4 SHF bands

Taking into account the wavelength and distances from the radiation sources, standard method of measurement shall be applied.

4.2 Instruments

4.2.1 Introduction

The measurement of exposure at the EMF, in the frequency range 10 kHz-300 GHz, requires big care for the spatial and time variability of the field to be measured.

For that it is necessary to use adequate instrumentation and a valid measurement set up.

It is very important to know the characteristics of the measurement instruments because some important factors have influence in their choice, for example the EMF in relation to the frequency or its harmonics, the characteristics of the field: if it is a reactive or radiative; type of polarization and modulation; number of radiant sources.

The problematic of the human body exposure to electromagnetic fields and at the power density, or other factory as the induct current in the body, are some of the most critical aspects for the protection or control that the engineer must resolve. In many cases we do not have a simple mathematical ratio between electric and magnetic field therefore, in this situation, each size must be distinguish measured.

The measurement instruments to use in this case are:

- specific instruments to measure directly the parameters of fields E or H;
- instruments to measure the temperature.

4.2.1.1 General

The base equipment of these instruments are:

- the probes;
- the connection cables, that transfer the signal from the probe to the reading and calculation unit;
- the reading and calculation unit.

4.2.1.2 Probes

Most probes are isotropic, or omnidirectional, to measure the energy from all directions.

The probes must respect the following conditions:

- provide only one parameter without answer to the spuries (i.e. the magnetic fields H are less important than the electric fields E under test);
- the dimension of the probe is very reduced, more less of $\lambda/10$ of the maximum frequency of the range in test;
- to have a known action at the variation of the environmental condition.

It is very important that the isotropic probe, during the measurement, is located perpendicularly to the antenna's polarization; in this condition we do not have coupling between the leg of the probe and EMF from the antenna. That is more evident when it is measuring medium wave signals.

4.2.1.3 Cables

The cables used to connect the probe at the reading and calculating instrument must be noise free and prevent coupling of the energy produced by the device under test (DUT) circuit and the measurement unit.

It is very important to note that it can be possible that the cables could turn the receiver to give RF power to the instruments, to bring about a change of the real value reading.

It is possible to resolve this problem by setting the cables, during the test, perpendicularly to the source.

4.2.2 Characteristics of the measurement instruments for electric and magnetic field

Generally the measurement of exposure to EMF is executed in the frequency dominion. We have two principal groups of instruments.

4.2.2.1 Wideband instruments types and specifications

With broadband instruments (see Fig. 2) we can measure the total field in a given frequency range (i.e. bandwidth), but it is not possible to distinguish the contribution of a single frequency source, when several source are radiating simultaneously.

FIGURE 2
Broadband instruments



Rap. 2037-02

The broadband instruments are made by sensors that can be non-isotropic to measure a single spatial component of the field, or can be isotropic to measure all components of the field in the same time. These instruments can measure the total level of the instantaneous EMF, or the RMS value or the average value in a time period, typically 6 min in accord to the law disposition.

The broadband instruments can be divided in the following classes, in function of the transducer's characteristic that is used:

- diode
- bolometer
- thermo coupler.

Those instruments can be used in both situations of near field and far field.

4.2.3 Narrow-band instrument types and specifications


The narrow-band instruments are selective in frequency and can measure the electromagnetic field amplitude at different frequencies. By means of non-isotropic sensor or antennas it is possible to evaluate the direction and the polarization of the field. Care must be addressed in the set up preparation since the high frequency EMF changes rapidly in space, especially in the presence of reflective objects like walls, earth, metallic poles and structures. It is important to observe that by changing the measurement point the detected field is completely different.

The measurement can be influenced from the antenna position or/and connection cables.

When the measurement of the EMF in high frequency is executed in the time domain, it is necessary to use instruments with appropriate characteristic of analysis (for frequency and resolution answer) to obtain good results in the spectral analysis by Fourier's transform.

In Fig. 3 we can see the block diagram of the measurement line for narrow-band base.

FIGURE 3
Block diagram of the measurement line

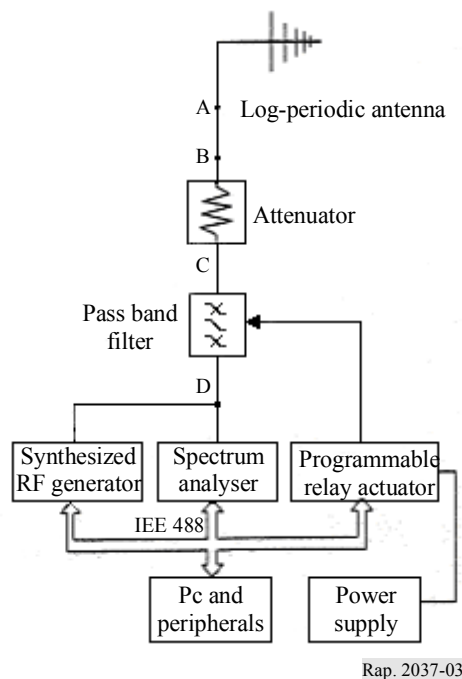


These instruments consist of the following fundamental elements:

- The sensor, or the antenna, that measure the intensity of electric field E otherwise the magnetic field H; for E use a dipole and for H use a loop.
- The transducer, that changes the answer of the sensor in a proportional value of E or H.
- The connecting calibrate cable.

- The selective receiver (see Fig. 4) (that measures the field intensity) through a tuning circuit displaying the signal in voltage received at a selected frequency. The spectrum analyser shows on the monitor the values of the voltage or the power in the frequency domain.

FIGURE 4

A selective receiver with spectrum analyser

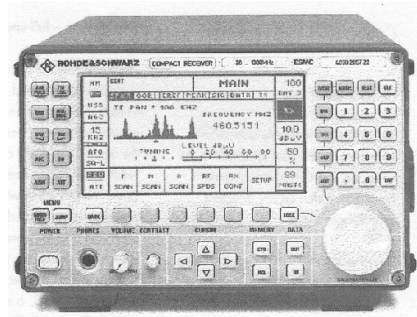

Rap. 2037-04

It is very important to use accuracy during these measurements, so that the measuring instruments do not disturb the device under test.

4.3 Comparison between predictions and measurements

The comparison between predictions and measurements indicate that results of the measurements are in good agreement with results obtained by theoretical computation. For more details, see Appendix 2.

5 Precautions at transmitting stations and their vicinity

This section outlines the precautions that should be taken at high-power broadcasting transmitting stations to control the potential risks due to RF radiation. These risks fall into two main categories, the first being the direct risk to health due to human exposure to high levels of RF radiation, including shocks, burns and the possible malfunctioning of medical implants. The second category comprises indirect risks where RF radiation could cause explosions, fires or interfere with the safe working of machines, cranes, vehicles, etc.

5.1 Precautions to control the direct health effects of RF radiation

Two groups of people are considered in terms of the precautions that can reasonably be taken. The first group is employees at, or regular official visitors to, transmitting stations. Whilst this group may be at a more frequent risk, the extent to which control measures can be applied is much greater than that for the second group, being members of the general public.

5.1.1 Employee (occupational) precautionary measures

5.1.1.1 Physical measures

Some form of protective barrier must be provided to restrict access to any area where either the basic biological limits are exceeded or contact with exposed RF conductors is possible. Access to such areas must only be possible with the use of a key or some form of tool. Mechanical or electrical interlocking should be provided to enclosures where access for maintenance is needed. Screening of equipment should be sufficiently effective to reduce the level of RF radiation.

Other physical measures such as warning lights or signs should also be used in addition to, but not instead of, protective barriers.

The risk of shock or burns from RF voltages induced on conducting objects, such as fences and support structures, should be minimized by efficient and properly maintained RF earthing arrangements. Particular attention should be paid to the earthing of any temporary cables or wire ropes, such as winch bonds, etc.

Where such objects need to be handled in an RF field, additional protection from shocks or burns should be provided by the wearing of heavy-duty gloves and through effective labelling.

5.1.1.2 Operational procedures

RF radiation risk assessments must be carried out by suitably trained and experienced staff at regular intervals and also when any significant changes are made to a transmitting station. The initial objective must include the identification of the following:

- the areas where people may be exposed to “derived” or “investigation” levels;
- the different groups of people, e.g. employees, site sharers, general public etc., who may be exposed;
- the consequences of fault conditions, such as leakage from RF flanges, antenna misalignment or operational errors.

An initial check on the RF radiation levels can be done by calculation or mathematical modelling, but some sample measurements should also be carried out for verification purposes. In most cases, however, measurements will be needed to determine RF radiation levels more accurately. The actual quantities to be measured (E field, H field, pfd, induced current) should be determined based on the specific circumstances. These include station frequencies, field region (near/far field) being measured and whether it is proposed to check compliance with basic restrictions (SAR) or only “derived/investigation” levels. These circumstances will also largely determine whether the three individual field components should be measured separately or whether an isotropic instrument should be used. RF radiation surveys should then be carried out by staff trained in the use of such instruments, following prescribed measurement procedures, and recording results in a specified format.

A nominated competent person should be made responsible for the identification and provision of suitable types within any organization or company. Such measuring instruments must always be used in accordance with manufacturers instructions and be subject to regular functional testing and calibration. Labels showing expiry dates must be fixed to instruments following such tests or

calibration. Records of calibration should be kept, including whether adjustments and/or repairs were needed on each occasion. This information should then be used to determine the interval between calibrations.

Systems of work should be implemented that not only ensure that RF radiation limits are not exceeded, but also minimize exposure in terms of time and number of employees. Maintenance work, in areas subject to access restrictions due to high RF radiation levels, should be planned around scheduled transmission breaks or radiation pattern changes where possible. However, there should always be a balance between exposure to RF radiation and other risks, such as working on masts at night, even when floodlit. Where necessary, transmitters should be switched to reduced power or turned off to allow safe access for maintenance or repair work.

Prohibited areas on transmitting stations must be clearly defined and marked, and “permit to work” systems should be implemented. Appropriate arrangements should be put in place for any systems, antennas, combiners or areas shared by other organizations. All staff who regularly work in areas with high levels of RF radiation should be issued with some form of personal alarm or RF hazard meter.

Records must be kept of exposure above specified RF radiation levels. Companies or organizations responsible for operating transmitting stations should monitor the health of staff who regularly work in areas with high levels of RF radiation and take part in epidemiological surveys, where appropriate.

Details of general policies and procedures relating to RF radiation safety should be included in written safety instructions and given to all appropriate staff. In addition, local instructions for each transmitting station should be issued to ensure compliance with such policies and procedures.

Safety training should also include the nature and effects of RF radiation, the medical aspects and safety standards.

5.1.2 Precautionary measures in relation to the general public

5.1.2.1 Physical measures

Similar considerations apply to the general public, as those detailed in § 5.1.1.1 for employees. Particular attention should be given to areas where RF radiation limits could be exceeded under fault conditions. Protective barriers should be provided in the form of perimeter fencing, suitably earthed where needed. Additional hazard warning signs will probably be necessary.

5.1.2.2 Operational procedures

Risk assessments, carried out under § 5.1.1.2, must take into account the possibility of members of the public having medical implants. A procedure for providing health hazard information to such potential visitors should be adopted with appropriate restricted access procedures. Basic RF safety instructions should be provided for regular site visitors.

The need to carry out RF radiation surveys beyond site boundaries must be considered, in particular where induced voltages in external metallic structures (cranes, bridges, buildings etc.) may cause minor burns or shock. In carrying out such surveys the possibility of the field strength increasing with distance, usually due to rising terrain, should be taken into account. Where necessary, a procedure for monitoring planning applications or other development proposals should be implemented.

An example which illustrates the text above is given in Appendix 3 (Fig. 4.3 and Fig. 4.4)

5.2 Precautions to control the indirect RF radiation hazards

Indirect effects of RF radiation, such as ignition hazards to flammable substances, may occur at levels well below the “derived/investigation” levels particularly at MF/HF. This is because flammable substances may be stored on a site having associated conducting structures, such as pipe work, that could act as a fairly efficient receiving antenna. Actual risks are, however, rare, but may include industrial processing plants, fuel storage facilities and petrol filling stations. Detailed evaluation is, however, far from simple. The general procedure recommended below is, therefore, based on progressive elimination. The detailed precautions adopted will however need to take account of any national standards or legislation in the country concerned.

An initial assessment should be carried out, based on practical, worst case estimates, of the minimum separation needed between a particular type of transmitter and a conducting structure to avoid such a hazard. The first step in doing this is to determine the minimum field strength that might present an ignition hazard for the particular transmitter frequencies in use. This is a function of the type of flammable substance and the perimeter of any loop formed by metallic structures, usually pipe work, and can most easily be determined from tables or graphs. The vulnerable area should then be determined from this minimum field strength by calculation, mathematical modelling or from tables/graphs.

If the vulnerable area, as determined above, contains any such sites on which flammable substances are stored, or if any are being planned, a more detailed assessment should then be made. This should be based on the actual dimensions of any metallic structures, the gas category of the flammable substance(s) being stored and the measured field strength. This detailed assessment should be carried out by calculation of the extractable power from the metallic structure to determine whether this exceeds the minimum ignition energy of the flammable substance. Should this be the case, then the extractable power should be measured and any necessary modifications to the structure and/or other safeguards implemented.

In a similar category to ignition hazards, is the possible detonation of explosive materials. This will very rarely be encountered but detailed guidance is available from national standards, such as BS 6657 in the United Kingdom. Other indirect effects that should be considered include interference to the safety systems of vehicles, machines, cranes etc. close to, or within the boundaries of, transmitting stations. The immunity of these systems is covered by electromagnetic compatibility (EMC) regulations (see Appendix 3).

Where necessary, precautions similar in principle to those described in § 5.1.2 may need to be applied.


Appendix 1

Examples of calculated field strengths near broadcasting antennas

1 Example A – Electric and magnetic field-strength plots

According to Section 3 numerical calculations of electric and magnetic field-strength distribution near broadcasting transmitting antennas can be done in order to check how the field strengths are at certain points or areas. This includes especially the near-field zone, where the field structure is generally very complicated. Calculations can also be done in order to verify the field contours (lines or surfaces with constant field strength) where relevant limiting values (levels) of EMF restrictions are kept. In this way it is possible (e.g. for planning purposes) to estimate how extended relevant zones may be, where protection measures may or must be performed.


In a technical document of the EBU [2] many calculation results are given. In the following Figures some calculation results of these examples (MF and HF broadcasting transmitting antennas) are given as plots.

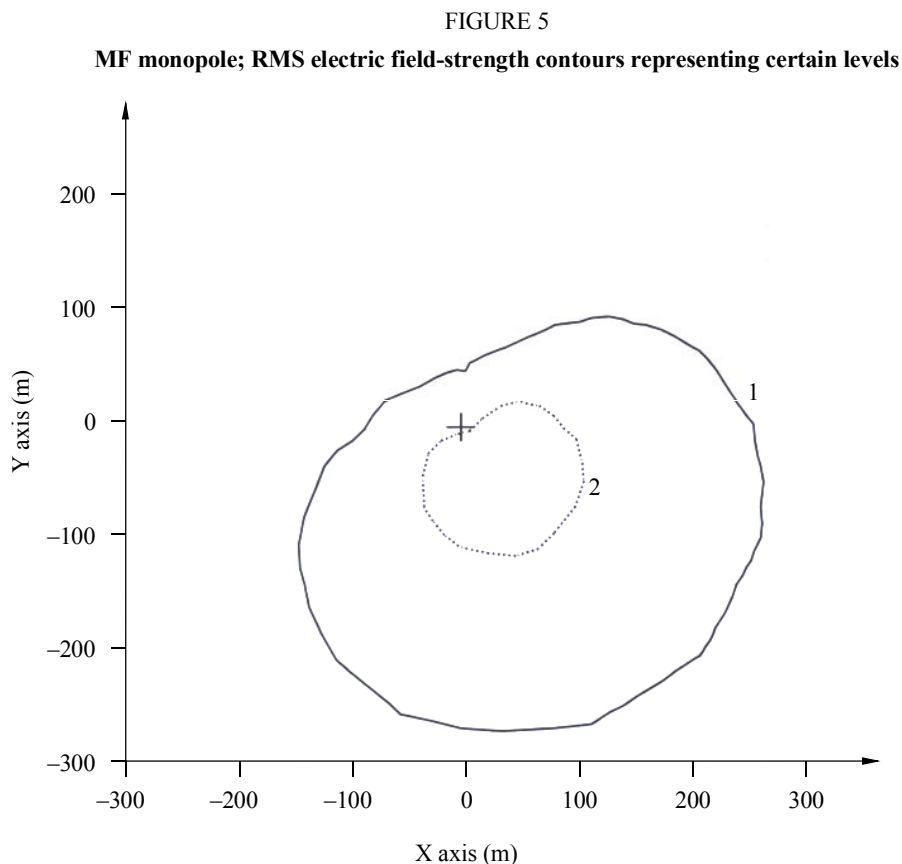

1: ICNIRP (general publication) = 60 V/m
 2: 158 V/m
 E_{max} : 449.8 V/m
 Frequency: 1 422 kHz
 Power: 600 kW
 Evaluation height: 1.5 m above ground level (agl)

FIGURE 6

MF monopole; RMS magnetic field-strength contours representing certain levels

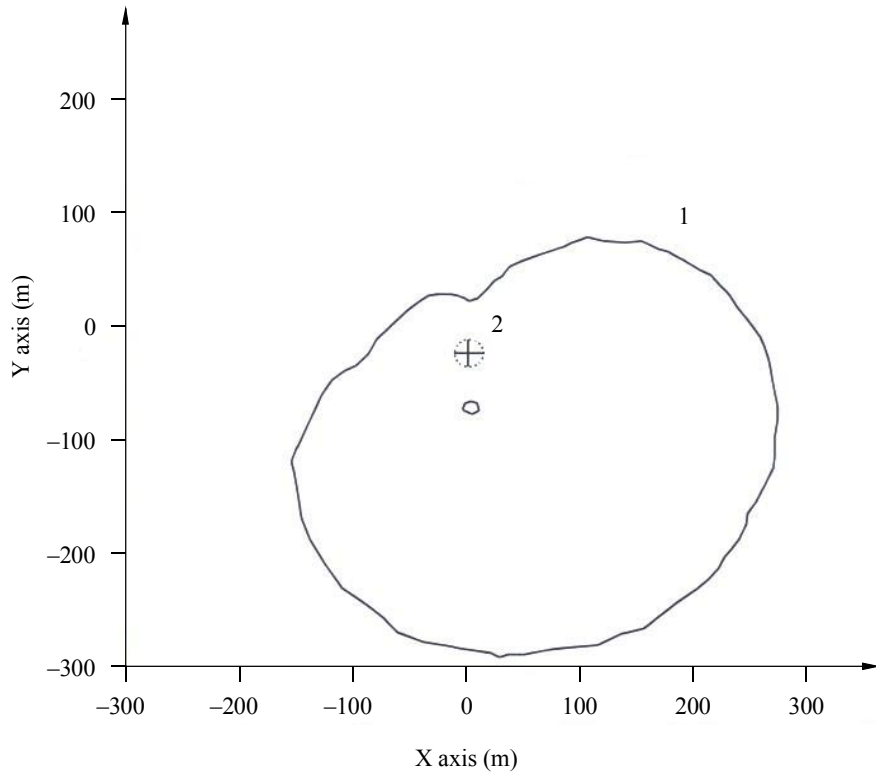


1: ICNIRP (general publication) = 0.16 A/m
 2: 1.3 A/m
 H_{max} : 1.6 A/m
 Frequency: 1 422 kHz
 Power: 600 kW
 Evaluation height: 1.5 m agl

Rap. 2037-06

FIGURE 7


HF curtain array; boresight plot for RMS electric field-strength values at 6 MHz and 500 kW (1.5 m agl)

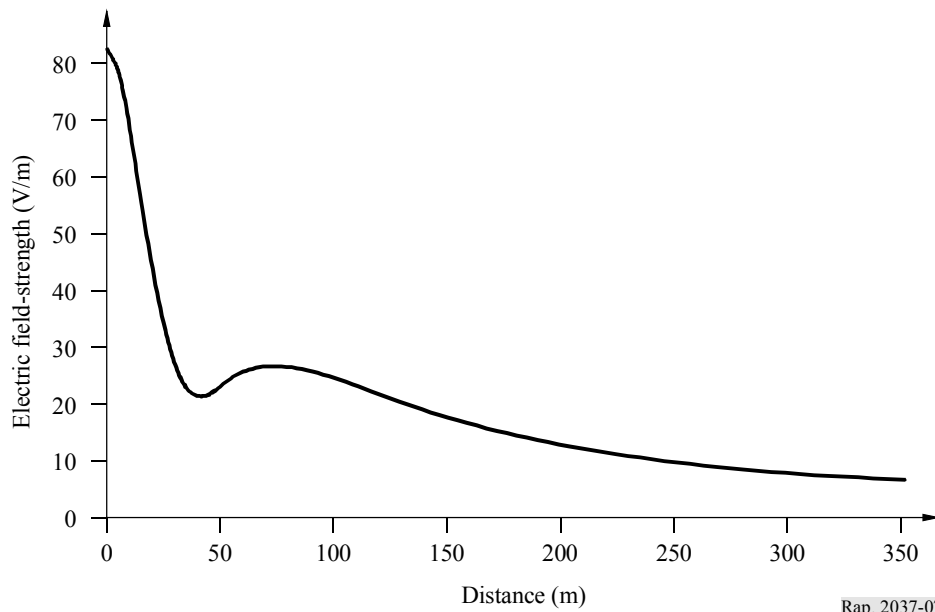

Rap. 2037-07

FIGURE 8

HF curtain array; RMS electric field-strength contours (V/m) representing certain levels

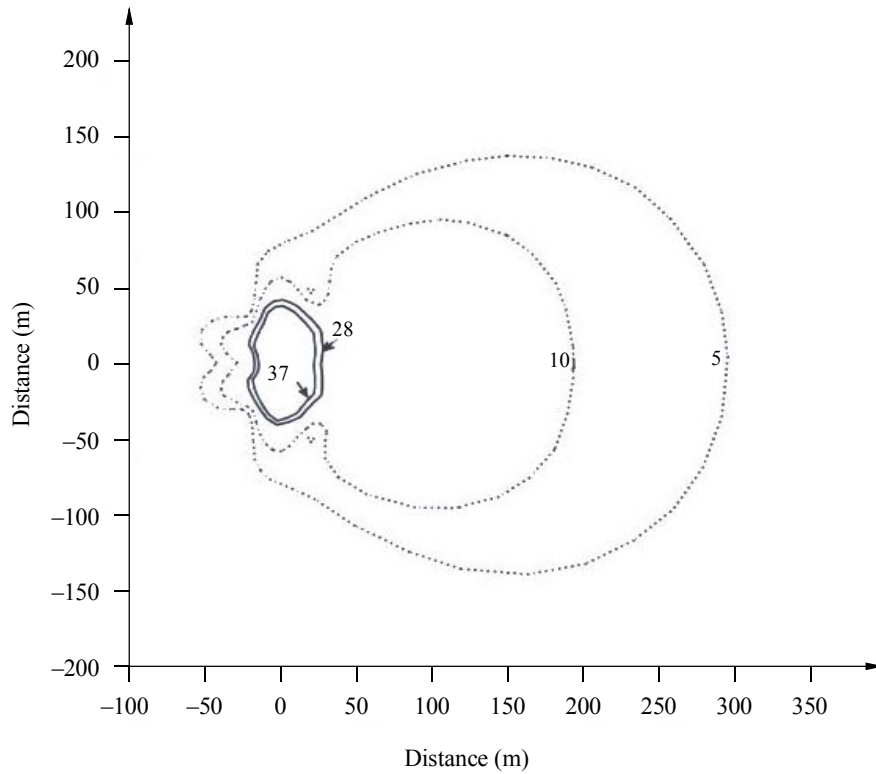


Power: 500 kW
Frequency: 6 MHz
Evaluation height: 1.5 m agl

Rap. 2037-08

FIGURE 9


HF curtain array; boresight plot for RMS magnetic field-strength values at 6 MHz and 500 kW (1.5 m agl)

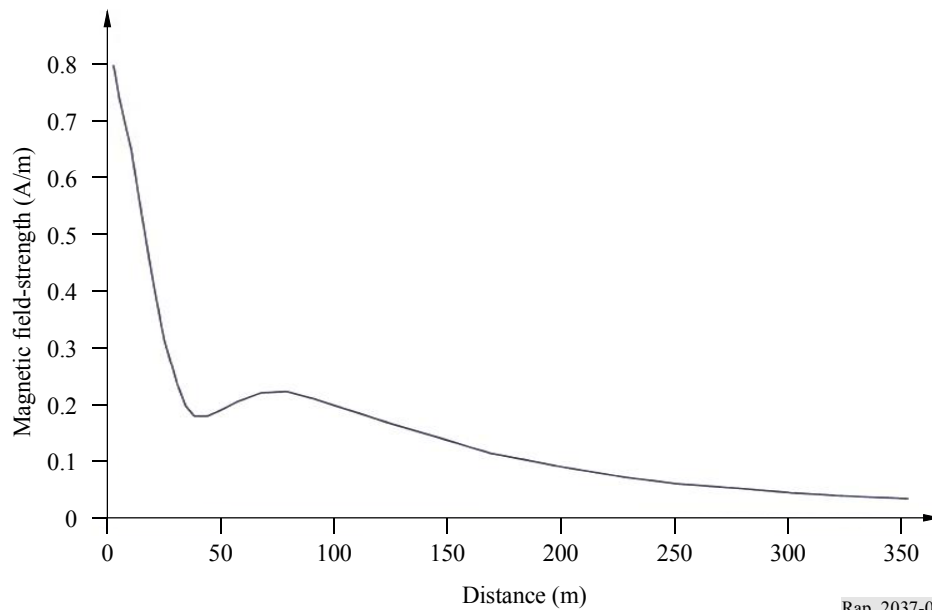

Rap. 2037-09

FIGURE 10

HF curtain array; RMS magnetic field-strength contours (A/m)
representing certain levels

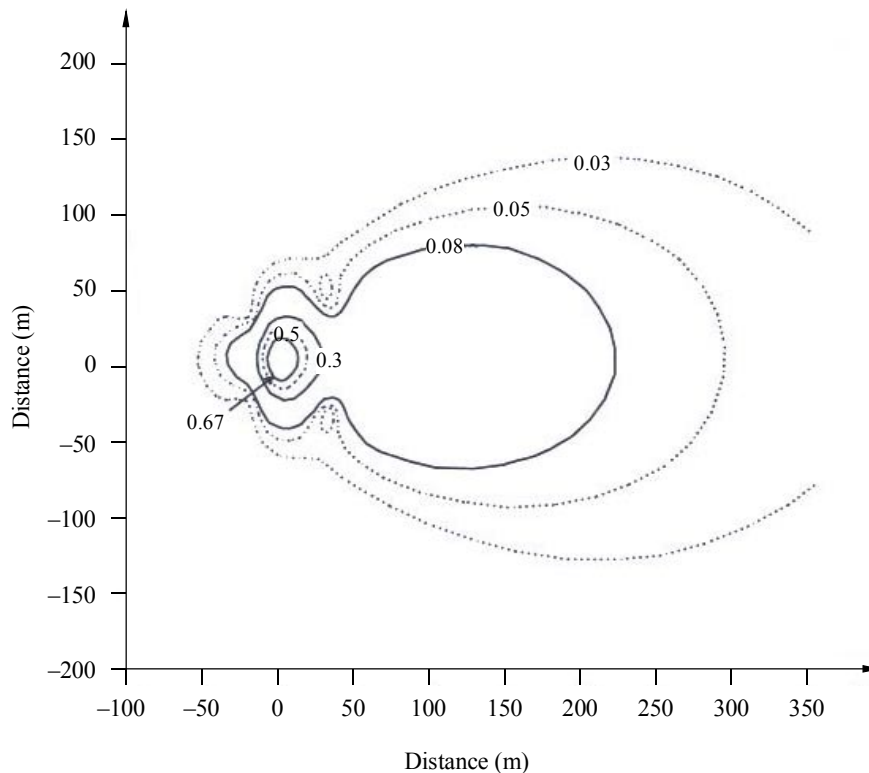

Power: 500 kW
Frequency: 6 MHz
Evaluation height: 1.5 m agl

Rap. 2037-10

2 Example B – Determination of the magnetic field strength in the near field zone of high-power MF/LF antennas

This example has the aim to determine magnetic field strength in the near-field zone of MF and LF mast antennas (monopoles), solving Hallen's integral equation.

In frequency bands below 10 MHz physical relations in the EMF are much more complex. In contrast to microwave frequencies, where the EMF has characteristics of the field in the far zone even at very short distances from the radiation source, and where the concept of the radiated power density (Poynting vector intensity) is very useful, in the MF/LF frequency band the field in the antenna vicinity is very complex. In fact, in the near field zone, the simple relationship between the electric and magnetic fields no longer exist: the two fields are not in phase and their ratio is not 377Ω . That fact additionally complicates the relationships in the EMF below 10 MHz.

Clearly, the measured field strengths will depend on the type of transmitting antenna, transmitter power and distance from the transmitting antenna. For example, in the case of high-power transmitter E-component, field strengths on a typical LF/MF site may range from a few V/m to over 250 V/m. Very close to the transmitting antenna the field strength may be of the order of 1 000 V/m.

3 Example C – Near electromagnetic field of HF transmitting curtain antennas

3.1 Introduction

This example deals with significantly more complicated antenna structures, referred to as curtain antennas. These antennas are very important for short-wave (HF) high-power transmitting purposes. They are, actually, arrays of horizontal dipoles arranged in a vertical plane.

The general trend towards increasing power and gain of transmitting antennas is very pronounced in HF broadcasting. Transmitter power of 500 kW and antenna gain (in the direction of the maximum of radiation) of over 20 dB (with respect to a half-wave dipole) has become almost standard in large transmitting centres for the global diffusion. A 500 kW transmitter with an antenna of a 20 dB gain produces an effective radiated power (ERP) of 50 MW.

In § 3.2, the numerical technique is briefly described which was used to compute near electric and magnetic fields of high-power antennas. Finally, in § 3.3, results are given for the fields in the vicinity of the HF curtain antennas.

3.2 Numerical analysis of wire structures

Calculations of the near fields of curtain antennas were done using program AWAS (Analysis of Wire Antennas and Scatterers), which is one of several programs developed at the School of Electrical Engineering, University of Belgrade, for the analysis of wire antennas and scatterers. Briefly, the program is based on formulating the so-called two-potential equation for the current distribution along the wires. This equation is solved using the MOM with the polynomial approximation for the current.

An arbitrary structure, located in a vacuum, and assembled from perfectly conducting straight wire segments is considered. According to the boundary conditions, on the wire surfaces, the tangential component of the total electric field must be zero, i.e.:

$$(\mathbf{E} + \mathbf{E}_i)_{\text{tan}} = 0 \quad (13)$$

where:

\mathbf{E} : electric field produced by the currents and charges of the wire structure

\mathbf{E}_i : impressed electric field, which models the excitation to the system.

The impressed field can be, for example, the electric field of a plane wave incident on the structure (when analysing scatterers or receiving antennas), or a field located in a small region at the antenna terminals, which models the generator driving the antenna (when analysing transmitting antennas).

The electric field produced by the wire currents and charges can be expressed in terms of the magnetic vector-potential, \mathbf{A} , and electric scalar-potential, V , as:

$$\mathbf{E} = -j\omega \mathbf{A} - \text{grad}V \quad (14)$$

where:

ω : angular frequency ($\omega = 2\pi f$).

The two potentials, in turn, can be expressed in terms of the densities of the surface currents (\mathbf{J}_s) and charges (ρ_s), which are related by the continuity equation. Next, the surface currents and charges are approximated by line currents and charges (thin-wire approximation), and the wire structure is divided into N segments (each of them having a local axis, s_m). Finally, the two-potential equation (also called the vector-scalar-potential equation) for the current distribution is obtained in the form

$$\sum_{m=1}^N \int_0^{h_m} \left[\mathbf{u}_p \cdot \mathbf{u}_m I_m(s_m) g(r_a) + \frac{1}{k^2} \frac{dI_m(s_m)}{ds_m} \text{grad } g(r_a) \right] ds_m = \frac{\mathbf{u}_p \cdot \mathbf{E}_i}{j \omega \mu_0} \quad (15)$$

where:

I_m : intensity of the current along a wire segment

$k = \omega \sqrt{\epsilon_0 \mu_0}$: free-space phase coefficient

$g(r_a) = \frac{1}{4\pi} \frac{\exp(-jk r_a)}{r_a}$: corresponding Green's function

r_a : approximate average distance between the point on the surface of the wire element ds_m and the field point.

Equation (15) is an integro-differential equation for the current distribution, and it can be solved only numerically. To that purpose, the general guidelines of the MOM are followed, and approximate the unknown function $I_m(s_m)$ by a series of known functions (basis functions), with unknown weighting coefficients. As the basis functions, the simple power functions are chosen, which amounts to the polynomial approximation of the current distribution, i.e.:

$$I_m(s_m) = \sum_{i=0}^{n_m} I_{mi} \left(\frac{s_m}{h_m} \right)^i \quad (16)$$


where:

h_m : segment length

I_{mi} : weighting coefficients.

Equation (15) cannot be satisfied exactly at all points along the wire segments, but only approximately. According to the MOM, a set of weighting functions is selected, and the inner products of equation (15) and these functions are evaluated. The weighting functions are taken to be pulses. Each pulse is a unity constant, defined on a short subsegment, and zero otherwise. A typical distribution of the pulses is shown in Fig. 11.

FIGURE 11
Typical distribution of pulse weighting functions
used in program AWAS

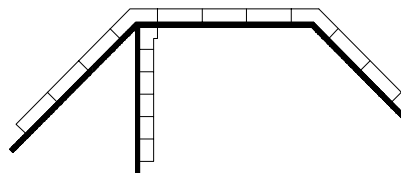

For a pulse defined on the subsegment (s_{p1}, s_{p2}) along the axis of the wire segment p , the evaluation of the inner product results in the equation (17):

$$\sum_{m=1}^N \sum_{i=0}^{n_m} I_{mi} \left\{ \int_{s_{p1}}^{s_{p2}} \int_0^{h_m} \mathbf{u}_p \cdot \mathbf{u}_m \left(\frac{s_m}{h_m} \right)^i g(r_a) ds_m ds_p + \frac{1}{k^2} \frac{i}{h_m} \int_0^{h_m} \left(\frac{s_m}{h_m} \right)^{i-1} [g(r_a)_{s_{p2}} - g(r_a)_{s_{p1}}] ds_m \right\} \\ + \sum_{i=0}^{n_p} I_{pi} \int_{s_{p1}}^{s_{p2}} \frac{Z'(s_p)}{j \omega \mu_0} \left(\frac{s_p}{h_p} \right)^i ds_p = \int_{s_{p1}}^{s_{p2}} \frac{\mathbf{u}_p \cdot \mathbf{E}_i}{j \omega \mu_0} ds_p \quad (17)$$

In this equation, \mathbf{u}_p is the unit vector of the wire segment p , and Z' is the impedance per unit length of a possible impedance loading distributed along the segment. When evaluated for all the pulses, equations of the form (17) comprise a system of linear equations in I_{mi} , which can be solved numerically.

Once the coefficients I_{mi} are known, the approximate current distribution along the wire segments is determined, and various characteristics of the wire structure can be evaluated. This part of the Report, deals primarily with the near electric and magnetic fields. The electric field can be evaluated in terms of the two potentials, in the similar way as when deriving the two-potential equation, i.e.:

$$\mathbf{E} = -j \omega \mu_0 \sum_{m=1}^N \sum_{i=0}^{n_m} I_{mi} \int_0^{h_m} \left[\mathbf{u}_m \left(\frac{s_m}{h_m} \right)^i g(r_a) + \frac{1}{k^2} \frac{i}{h_m} \left(\frac{s_m}{h_m} \right)^{i-1} \text{grad } g(r_a) \right] ds_m \quad (18)$$

The magnetic field can be expressed in terms of the magnetic vector-potential as:

$$\mathbf{H} = \frac{1}{\mu_0} \text{rot } \mathbf{A} \quad (19)$$

When this potentials is expressed in terms of the wire currents, one finally obtains:

$$\mathbf{H} = - \sum_{m=1}^N \sum_{i=0}^{n_m} I_{mi} \int_0^{h_m} \left(\frac{s_m}{h_m} \right)^i \mathbf{u}_m \times \text{grad } g(r_a) ds_m \quad (20)$$

3.3 Near electric and magnetic fields of curtain antennas

There is a variety of high-power transmitting antennas used in the HF range (short waves), like horizontal dipoles (usually forming a directive array), rhombic antennas, and vertical monopoles. The target of the investigation are arrays of horizontal dipoles, arranged in a vertical plane, known as curtain antennas, as this kind of arrays are planned to be used in the new short-way transmitting centre of Radio Yugoslavia, located at Stubline near Belgrade. The dipoles in a curtain array are usually half-wave dipoles, either simple, or folded, fed by currents of approximately equal amplitudes (but sometimes of different phases) to produce the desired radiation pattern. The array usually has a passive reflector, which in most practical cases consists of a wire mesh (aperiodic

reflector), but it can also be an array of tuned dipoles. Curtain arrays are labeled H(R)(S) $m/n/h$, where H denotes an array of horizontal dipoles arranged in a vertical plane; R denotes a reflector (if present); S denotes a phase shift (if present) between the currents feeding adjacent collinear dipoles in order to shift the azimuth of the main beam; m denotes the number of collinear dipoles in each row; n denotes the number of parallel dipoles stacked vertically (usually at a distance of one-half wavelength), i.e., the number of rows (bays); and h denotes the height of the lowest row above the ground (in wavelengths).

Curtain arrays have excellent properties, including a high gain (more than 20 dB), i.e., a highly directive radiation pattern, and high power-handling capabilities (up to 500 kW). Hence, they play a very important role in large HF transmitting centres. The central problem in this Report is developing an accurate and efficient technique for the evaluation of these fields.

The antenna field of the new HF centre of Radio Yugoslavia has a total of 15 horizontally polarized antennas. Two of them are quadrant antennas, with an omnidirectional characteristic, and thirteen are dipole curtain antennas (Fig. 12). Seven curtain antennas contain 16 folded dipoles each, arranged in four bays of four elements (HRS 4/4/ h), while six curtain antennas contain two folded dipoles each, arranged in one bay (HR 2/1/ h). All curtains have an aperiodic reflector, made of thin horizontal wires. The centre has two transmitters. The power of each transmitter is 500 kW (unmodulated carrier), and it is possible to simultaneously transmit two programs towards different destinations. The transmitters are connected to corresponding antennas through an antenna switching field, which is located in a room next to the transmitter hall. The layout of the antenna field, with the building with transmitters, is shown in Fig. 13. Figure 14 shows details of one antenna (B12).

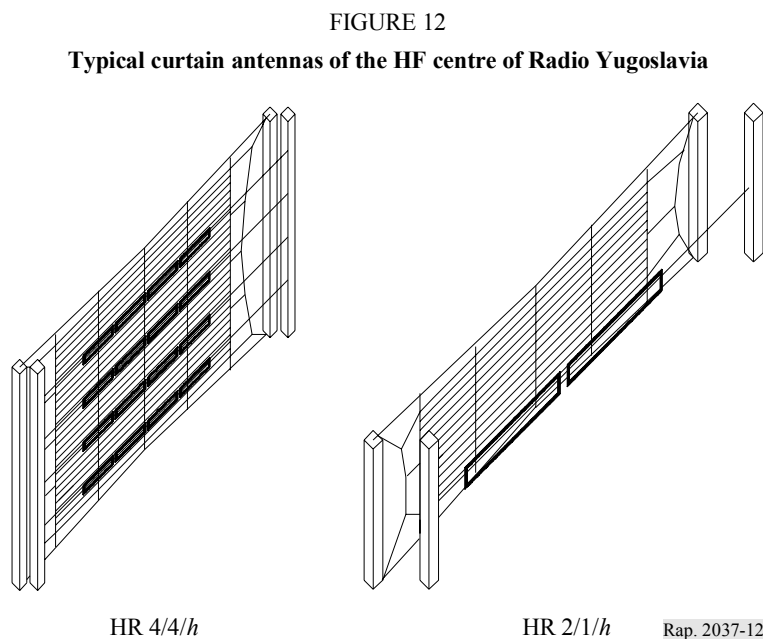


FIGURE 13
 Layout of the antenna field of the HF centre of Radio Yugoslavia


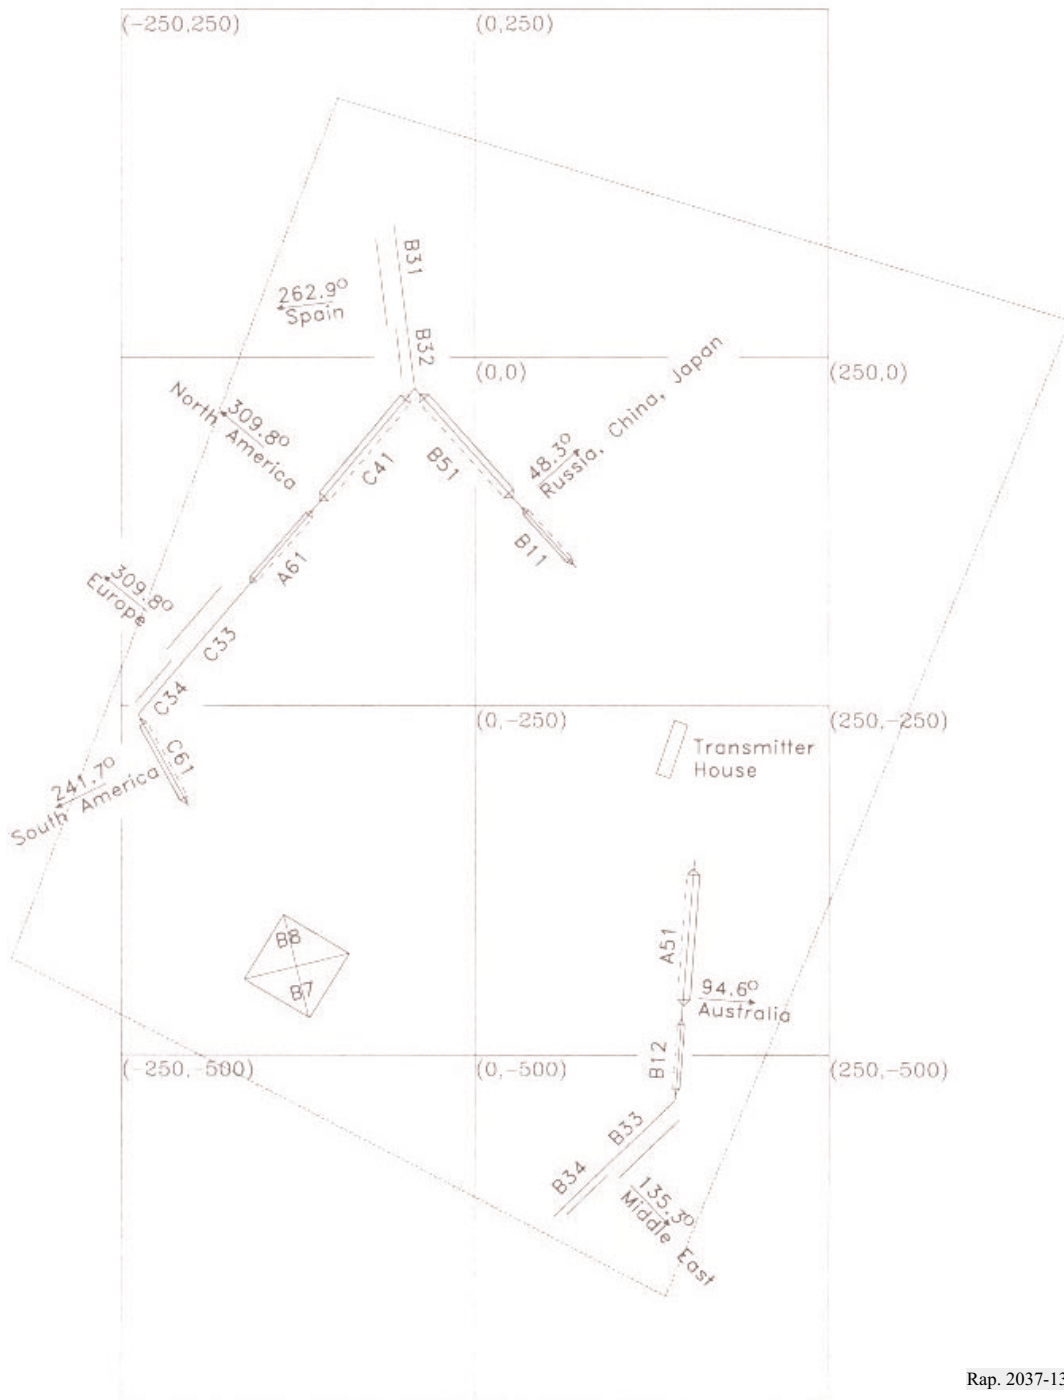


FIGURE 14


Detailed drawing of the dipole curtain antenna B12 (HRS 4/4/1)
of the HF centre of Radio Yugoslavia

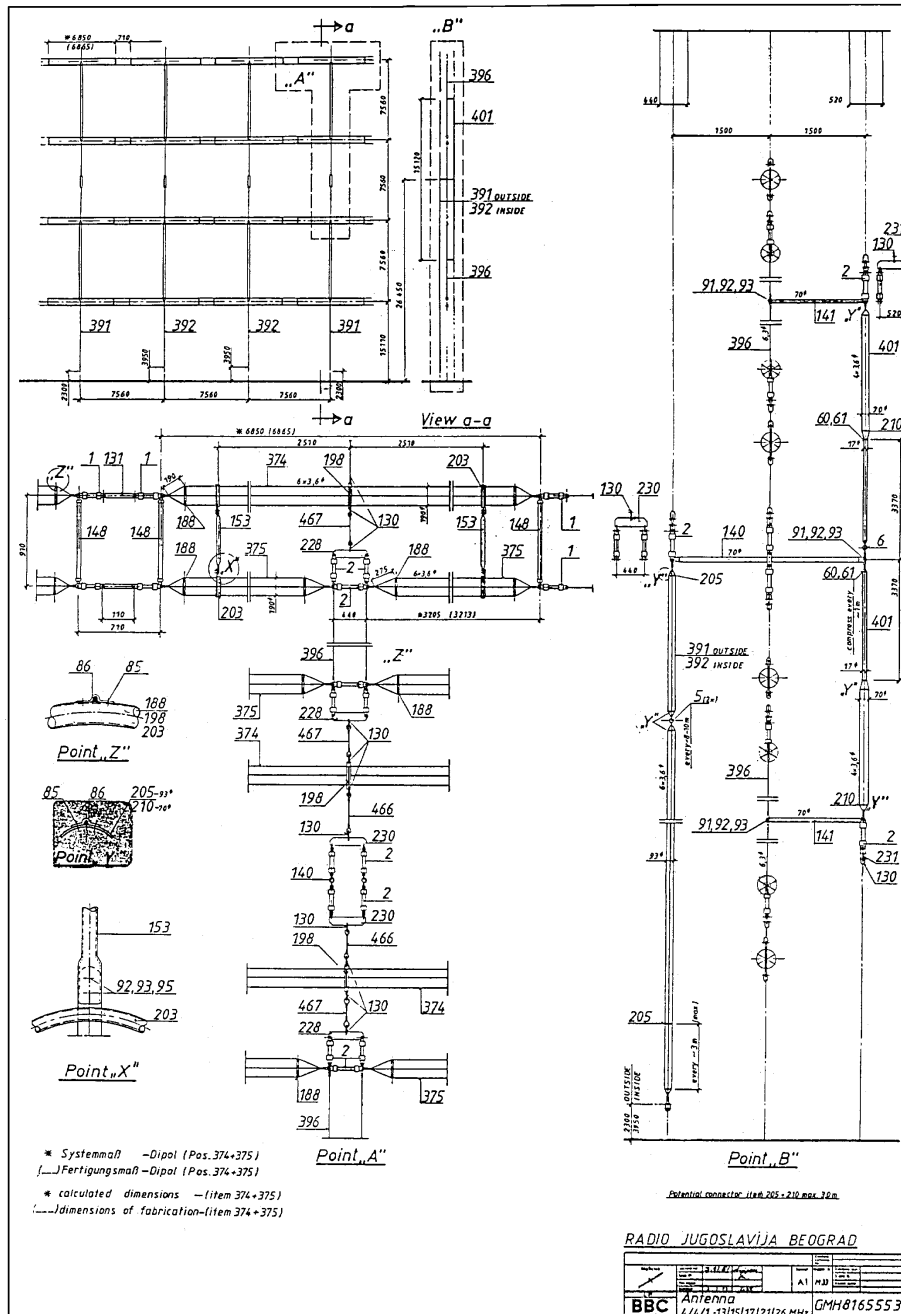

In the literature, there are few papers dealing with the calculation of the electric and magnetic fields of HF curtain antennas, but all of them are based on the sinusoidal approximation of the current distribution along dipoles, and on the assumption that the currents feeding dipoles have identical amplitudes. The goal is to provide a more rigorous analysis, using a more accurate approximation for the current distribution, and taking into account the coupling between the elements of the array, i.e., by feeding the elements by equal-amplitude voltages.

It has been shown experimentally (and confirmed theoretically using the sinusoidal approximation for the current distribution) that approximating the real soil by a perfectly conducting plane yields accurate results. This simplification is important, as it allows program AWAS to be used directly, without any modifications, as it can treat antennas only above a perfect ground. The present analysis was also expedited by taking simple dipoles instead of folded dipoles. This approximation was established to yield accurate results. The length of a simple dipole is taken to be somewhat shorter than half-wavelength at the design frequency, based on data taken from the dimensions of the actual curtains. The distance between feeding points of adjacent antennas is always half-wavelength, both horizontally and vertically. The distance between the dipoles and the reflector is exactly quarter-wavelength. The reflector was modelled by introducing negative images (in the vertical plane) of the original dipoles. The distance between the original dipoles and their respective images is thus half-wavelength. Figure 15 shows AWAS models of typical curtain antennas of the HF centre of Radio Yugoslavia.

FIGURE 15
AWAS model of a) the HRS 4/4/h antenna, and b) the HR 2/1/h antenna

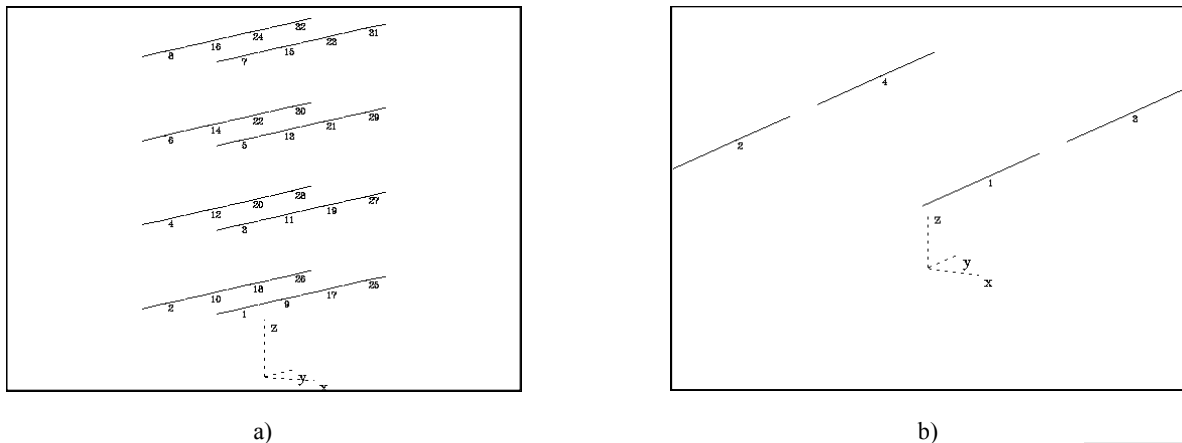


Rap. 2037-15

The near electric and magnetic fields were evaluated in the direction of the maximum of the radiation pattern (as the field in the direction of side lobes was found to be substantially weaker). The fields were evaluated at elevations of $z = 2$ m, for evaluation of radiation hazards for the staff of the centre, who may walk on the open field of the centre, and $z = 5$ m for the general population, taking into account possible dwelling in two-level houses.

Analysis results were first compared with the results for a HRS 4/4/1 antenna. The operating frequency of the antenna is 15.245 MHz, and the fed power is 500 kW. Figure 16a) shows the results for the “equivalent” Poynting vector, evaluated by AWAS, when the dipoles are assumed to be fed by identical currents. Figure 16b) shows the same results, but taking the dipoles to be fed by identical voltages, along with measured data at $z = 2$ m. The agreement between the theoretical and experimental data is fair. It is obvious that feeding the antenna with equal voltages results in a better prediction of the actual field, in particular near the dip at 70 m distance from the antenna.

FIGURE 16

The “equivalent” Poynting vector of the HRS 4/4/1 antenna evaluated by AWAS when dipoles are fed by a) identical currents, and b) identical voltages, along with experimental data (dots)

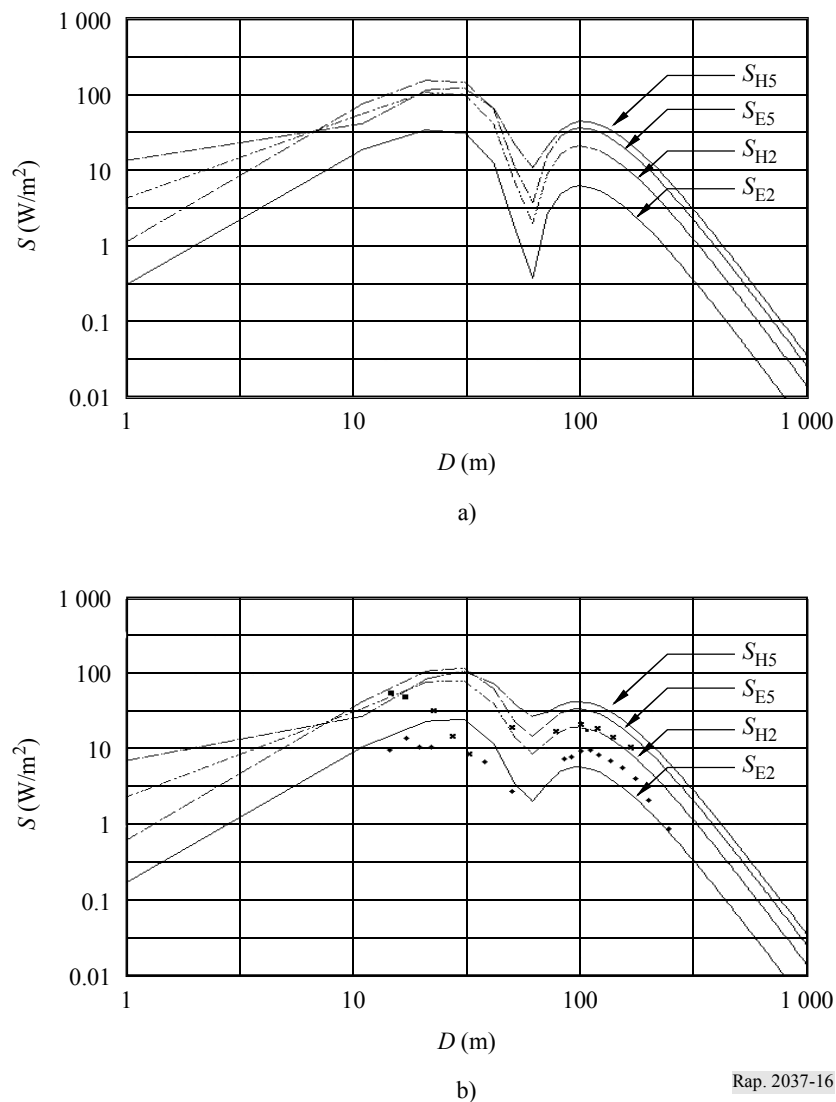

Gaining a confidence in the numerical technique used to calculate the near fields, the fields of all the curtain antennas of the new centre of Radio Yugoslavia have been evaluated. Two representative examples are shown in Figs. 17 and 18.

FIGURE 17

The “equivalent” Poynting vector of antenna A51 (HRS 4/4/0.5), operating at 9.63701 MHz. The safe distance from the antenna for the centre staff is 50 m, and for the general population is 300 m


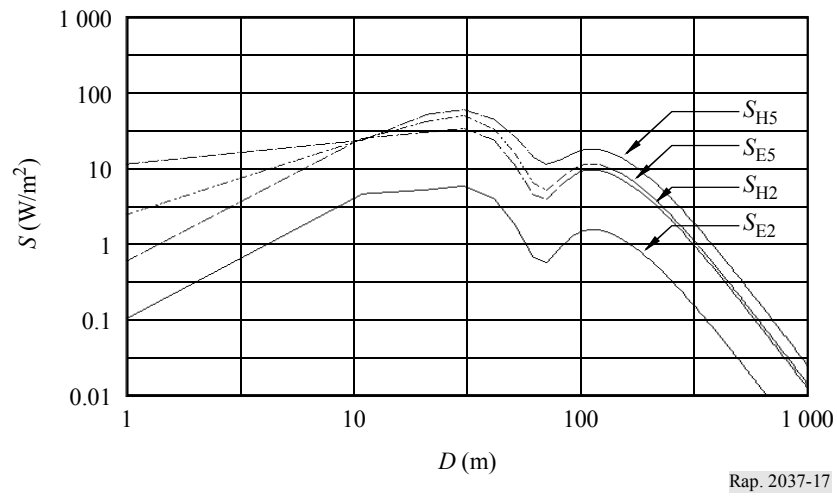


FIGURE 18

The “equivalent” Poynting vector of antenna C34 (HR 2/1/0.5), operating at 10.67996 MHz. The safe distance from the antenna for the centre staff is 70 m, and for the general population is 130 m

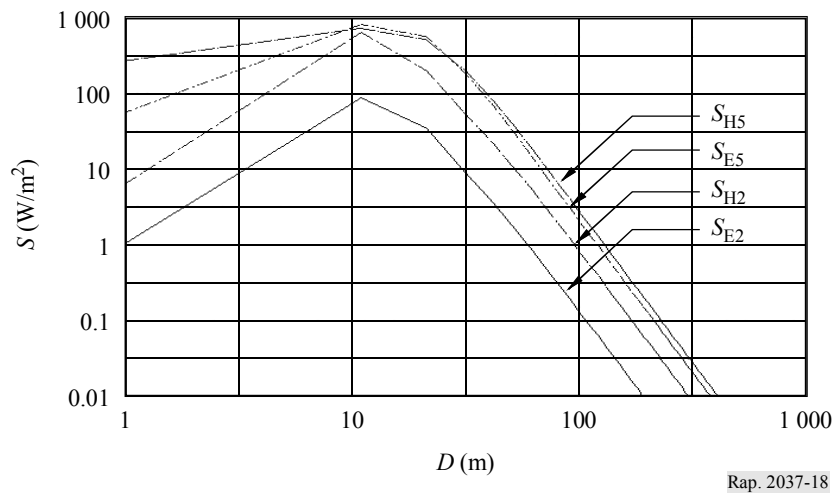

4 Conclusions

Near electric and magnetic fields in the vicinity of high-power transmitting HF curtain antennas have been investigated theoretically, using program AWAS. The theory was applied in particular to antennas of the new centre of Radio Yugoslavia. Safety zones for humans in the vicinity of these antennas were determined. The results for the near fields of curtain antennas are presented for the first time using a rigorous theory, and they are found to be in good agreement with experimental data published elsewhere.

Appendix 2

Comparison between predictions and measurements


1 Foreword

Simulation and measurements have been separately performed by different personnel without mutual communications in order to avoid reciprocal influences in work and in results.

Antenna system has been only partially simulated as it is particularly complex (see § 1.1 for antenna model).

Measurements and predictions have been performed on an antenna system, represented in Figs. 19 and 20, capable to correctly operate in the short wave band, comparison were made at 13 MHz and 18 MHz.

FIGURE 19
Antenna system

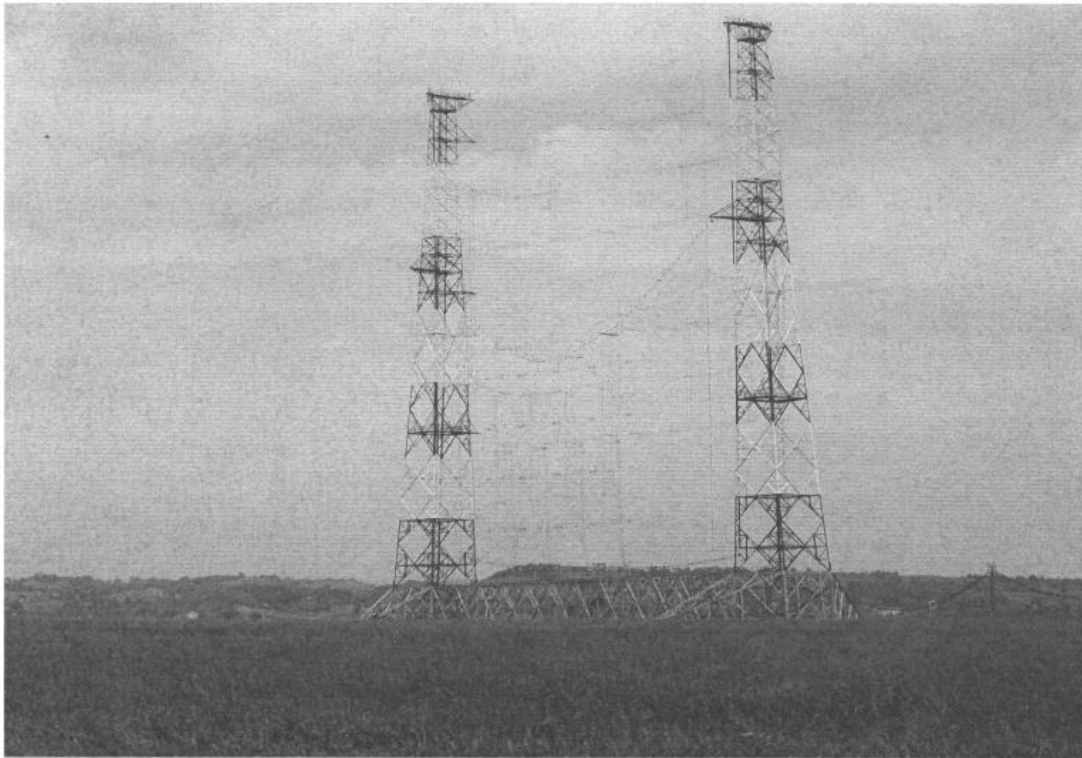


Rap. 2037-19

1.1 Model used for antenna system

The antenna system, shown in Fig. 19, is made of a horizontally polarized array of 16 folded dipoles disposed in front of a reflector realized by a wired network. Dipoles are fed by bifilar lines forming a complex impedance matching network; all bifilar lines of the impedance matching network,

represented in Fig. 20, are mainly vertically disposed (orthogonally to dipoles); some horizontal lines are relatively short and are orthogonally disposed both to dipoles and feeders, along the direction of propagation. At the antenna base are disposed other bifilar lines used to split the RF power among the four dipoles “columns”.

FIGURE 20
Matching and feeding network

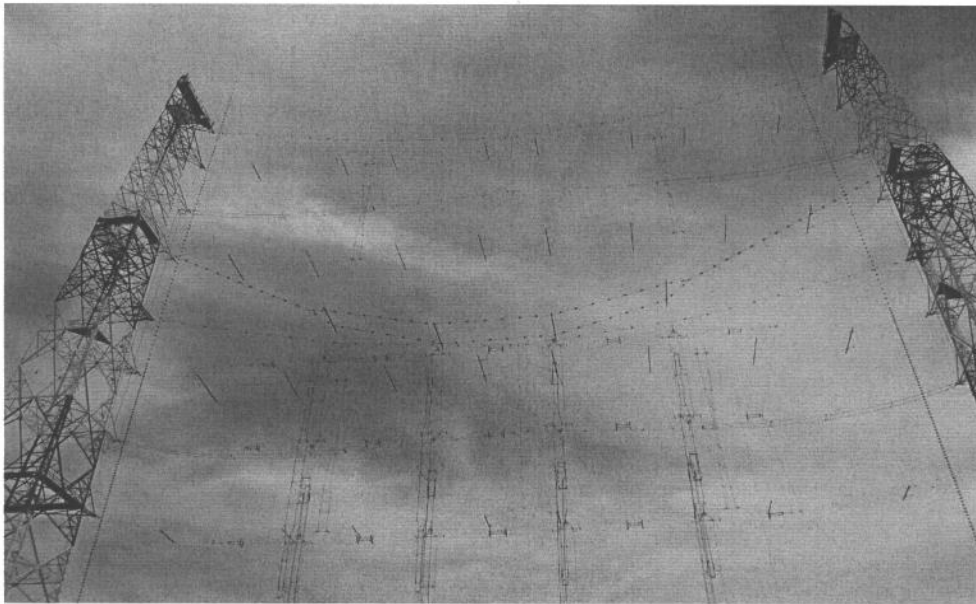

Rap 2037-20

In order to simplify the model and avoid unnecessary details and consequent longer calculation time, the entire system has been modelled as a simple 16 dipoles array as in Fig. 21, each fed by its own voltage generator correctly phased with all the others, with no need of a matching/feeding network. Furthermore, each folded dipole, physically realized by a couple of parallel wires folded at the edges, has been modelled as a single wire folded dipole, of an adequate section in order to obtain the identical value of impedance.

Finally, each dipole has been represented by 24 segments, each of a length not more than $\lambda/20$, as in Fig. 22.

1.2 Advantages and limitations of the implemented model of antenna system

The most important advantage is the extreme simplicity of the model realized versus the complexity of the real antenna system. Thanks to this model, it is possible to obtain a relatively low calculation time (about ten minutes in a 2 GHz Pentium 4).

Another advantage is the possibility of easily adjusting the model, if necessary, in order to better represent the real system. In fact, generally the result of a first comparison between simulations and measurements represent a good feedback to perform some adjustments on the first model. The most

important limitation in the simple model adopted is the impossibility to correctly take into account the contribution of the complex matching/feeding network to the x, y, z components of the fields. In fact a certain amount of power is radiated by bi-filar matching lines that work in standing wave regime. For this reason in the result of prediction the vertical component of E field does not appear (z component), as well as the horizontal component in the direction of propagation (y component), except in some cases where the values are quite low; a similar behaviour is visible for x component of H field. That is because the prediction was made without considering vertical radiators and radiators in the direction of propagation. In the measurements results, on the contrary, both the vertical (z) and the horizontal (y) components of E field are present, as well as the horizontal (x) component of H field, causing some problems in a direct comparison. The most reasonable thing to do is to consider these two components as generated by the amount of power that does not reach the dipoles array; their contribution to the measured field should be considered inside the horizontal (x) one in the result of simulation. In other terms, the horizontal contribution (x) resulting from the simulation must be compared with the global result of the measurements, obtained as square root of the sum of the square of contributions measured on x, y, z axis.

FIGURE 21

Dipoles array model and its orientation in the three-axis system X, Y, Z. Each dipole is fed by its own voltage generator, in phase with all the others. Contributes E_x , E_y , H_z , H_x , H_y , H_z of E and H fields in the evaluation point have the same orientation of the axis X, Y, Z


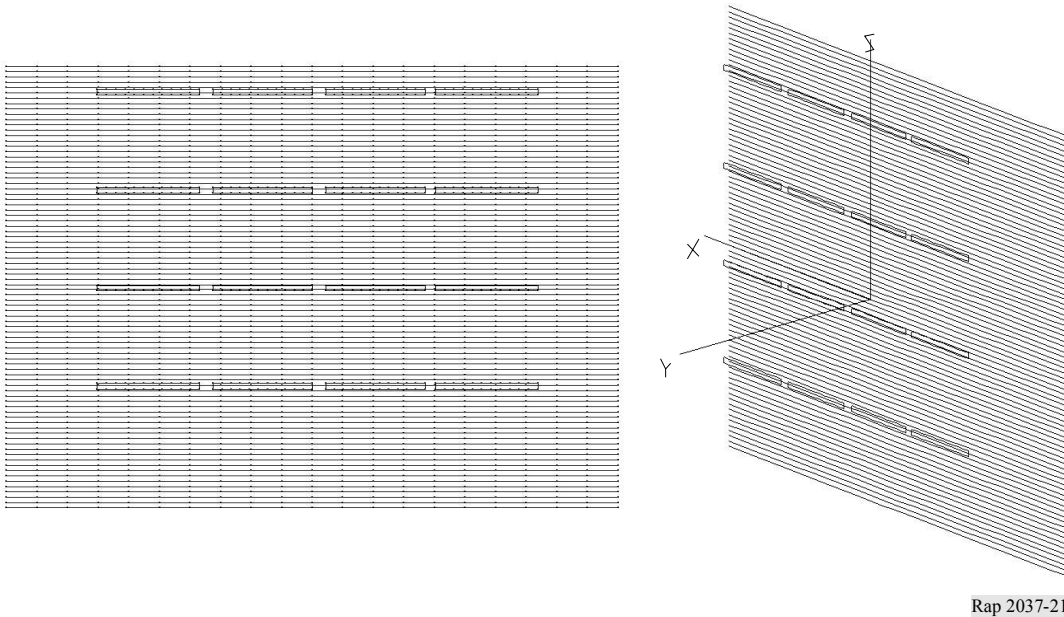


FIGURE 22

Single dipole model. Dipole is modelled by 24 segments each shorter than $\lambda/20$. Excitation is applied at the centre of the upper or lower arm, at the middle point of the central segment



Rap 2037-22

2 Comparison between prediction and measurements

2.1 13 MHz

2.1.1 Predictions


2.1.1.1 Notes about the model

In order to best fit the previously described model to the real antenna system, it is necessary to know the right amount of power at the input of each dipole, taking into account losses in transmission line and losses.

In order to apply the appropriate voltage value at each dipole, in the simulation the input impedance of each dipole has been calculated. The values are represented in Fig. 23.

FIGURE 23

Input impedance of dipoles obtained from simulation, normalized to 600 Ω .
Note the little - but not inexistent - dispersion of resistance values near 600 Ω

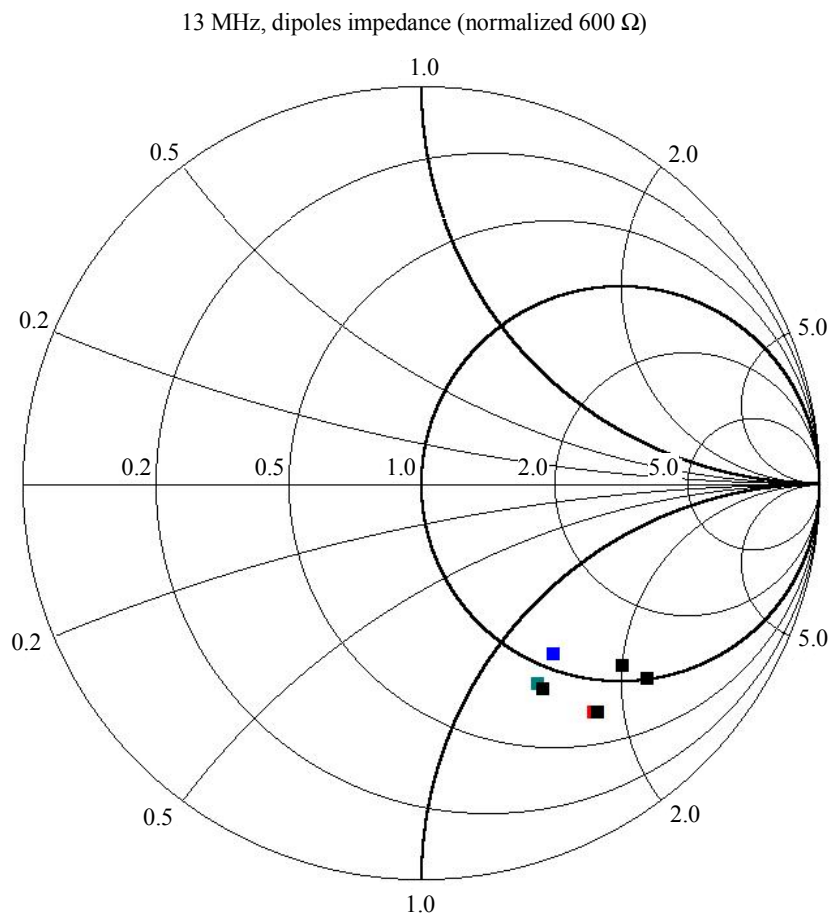


Then, for each dipole has been adopted a common value of resistance equal to 600Ω this being the average value obtained from the simulation. Note that this decision may be the cause of inaccuracy in the prediction's results.

In order to compensate the mismatch mainly due to the reactive component and the consequent reflection of power towards the transmitter, an adequate increase of power has been considered. Consequently, an adequate voltage has been applied at each dipole.

2.1.1.2 Far field evaluations


In order to best compare the behaviour of the model with real antennas, given in Figs. 19 and 20, the radiation diagrams were calculated. The results are shown in Fig. 24 (horizontal plane), Fig. 25 (vertical plane), Fig. 26 (frontal view).

FIGURE 24
Radiation diagram on horizontal plane

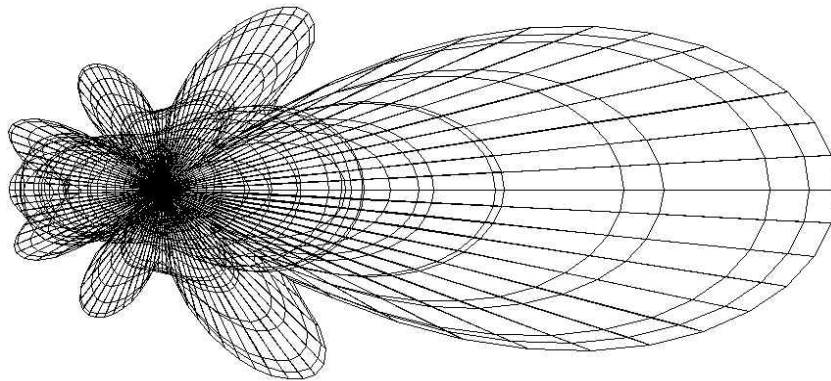


Rap 2037-24

FIGURE 25
Radiation diagram on vertical plane

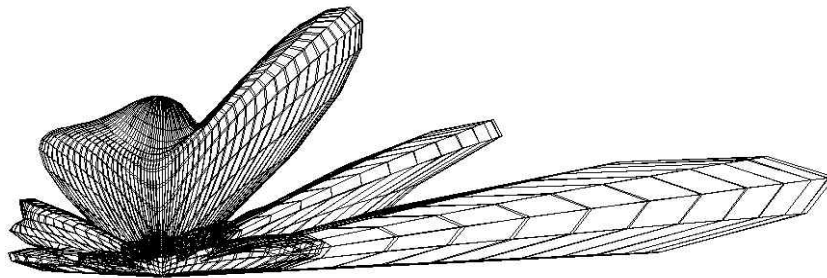

Rap 2037-25

FIGURE 26
Radiation diagram, front view

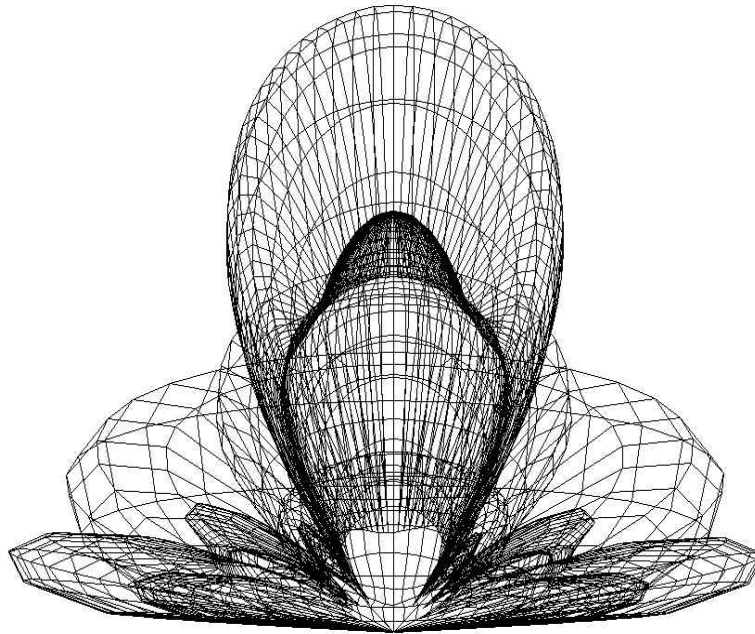


Rap 2037-26

2.1.1.3 Results of prediction of the field strength in the near zone

Prediction was made calculating the x , y , z components of E and H fields in the direction of the antenna's maximum gain (Y axis) at 2 m over terrain (Z axis = 2). The calculated values are represented in Fig. 27 (E field) and Fig. 28 (H field). The strong influence of the terrain both in the evaluations and in the measurements may introduce an additional difference between the two results. In order to show the strong influence of terrain, the E and H fields values have also been calculated varying the height of the evaluation point over the terrain (Z axis) from 0 up 9 m at a fixed distance of 60 m ($Y = 60$). The behaviour is illustrated in Fig. 29 (E field) and Fig. 30 (H field).

FIGURE 27
 Calculated E field strength in the near zone

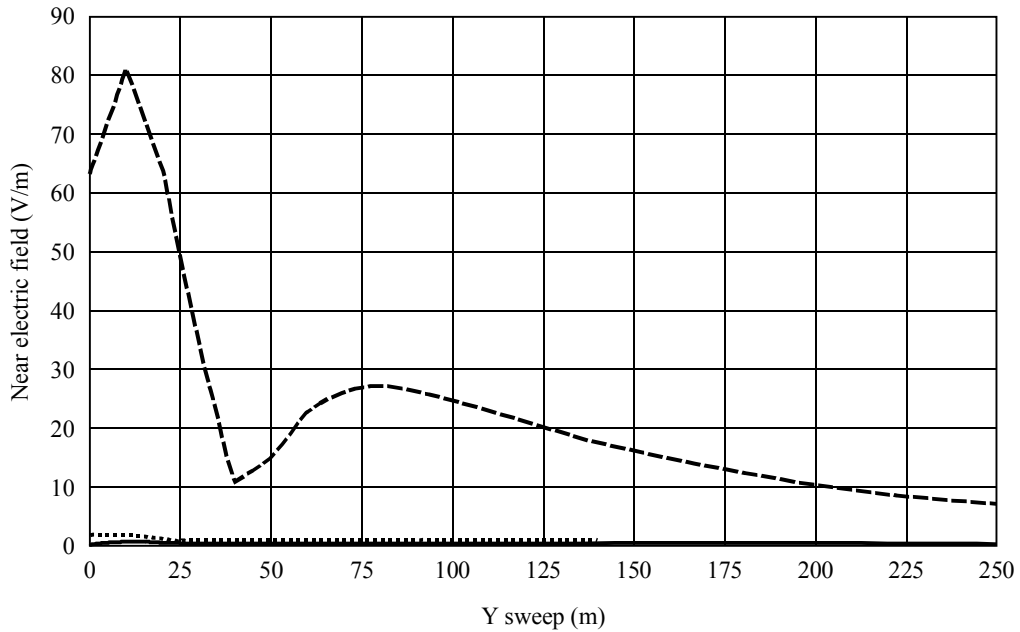


13 MHz, near electric field versus distance. Transmitter power: 225 kW at antenna connector.
 Height: 2 m over terrain

- Near electric field, mag (X), Y sweep, constants: X = 0, Z = 2; CORT13
- Near electric field, mag (Y), Y sweep, constants: X = 0, Z = 2; CORT13
- Near electric field, mag (Z), Y sweep, constants: X = 0, Z = 2; CORT13

Rap 2037-27

The most important contribute is the x component. On the horizontal axis is represented the distance in metres from antenna (Y sweep). Z is fixed at 2 m (height over terrain). The intensity of E field's components is represented in V/m on vertical axis.

FIGURE 28
Calculated H field strength in the near zone

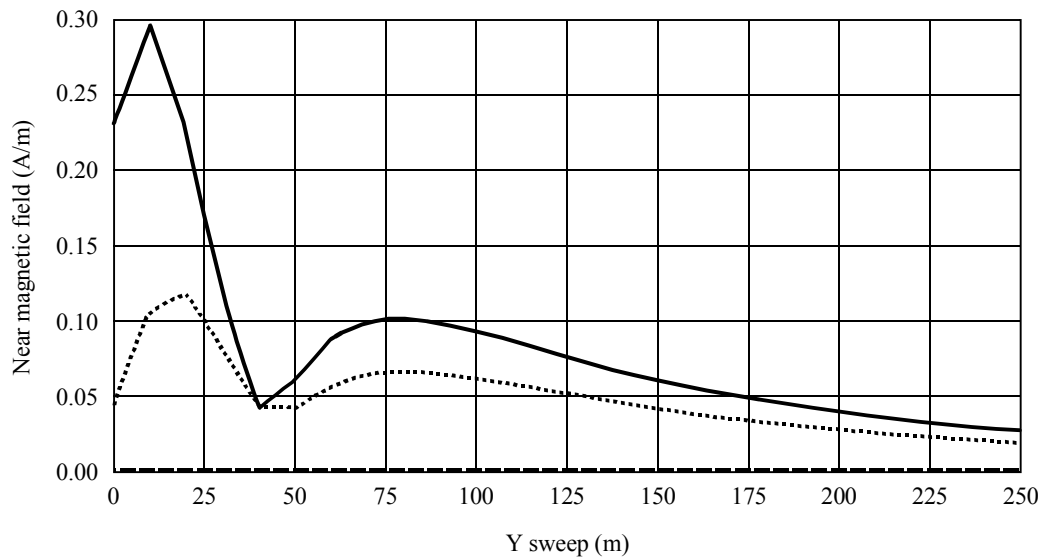

13 MHz, near magnetic field versus distance. Transmitter power: 225 kW at antenna connector. Height: 2 m over terrain


- Near magnetic field, mag (X), Y sweep, constants: X = 0, Z = 2; CORT13
- Near magnetic field, mag (Y), Y sweep, constants: X = 0, Z = 2; CORT13
- Near magnetic field, mag (Z), Y sweep, constants: X = 0, Z = 2; CORT13

Rap 2037-28

The main contribute is y component. The z component is lower, while x component is 0. On horizontal axis is represented the distance in metres from antenna (Y sweep). Z is fixed at 2 m (height over terrain). The intensity of H field's components is represented in A/m on vertical axis.

FIGURE 29

Calculated E field strength at a distance of 60 m from antenna (Y = 60)
at different heights between 0 and 9 m (Z sweep)

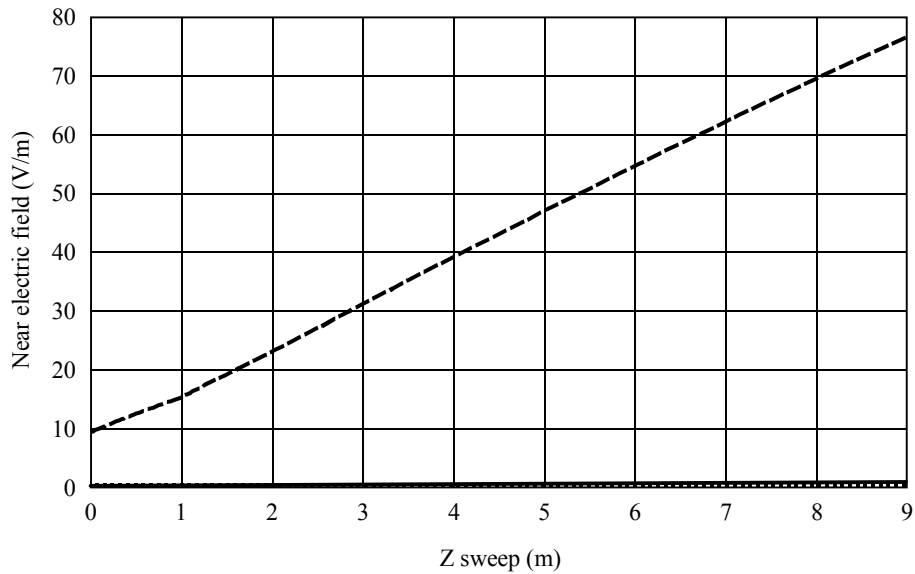


13 MHz, near electric field versus height @ 60 m from antenna.
Transmitter power: 225 kW at antenna connector.

- Near electric field, mag (X), Z sweep, constants: X = 0, Y = 60; CORT13
- Near electric field, mag (Y), Z sweep, constants: X = 0, Y = 60; CORT13
- Near electric field, mag (Z), Z sweep, constants: X = 0, Y = 60; CORT13

Rap 2037-29

It is evident the strong relationship between E values and height (only x component of E field is present).

FIGURE 30
 Calculated H field strength at a distance of 60 m from antenna (Y = 60)
 at different heights between 0 and 9 m (Z sweep)

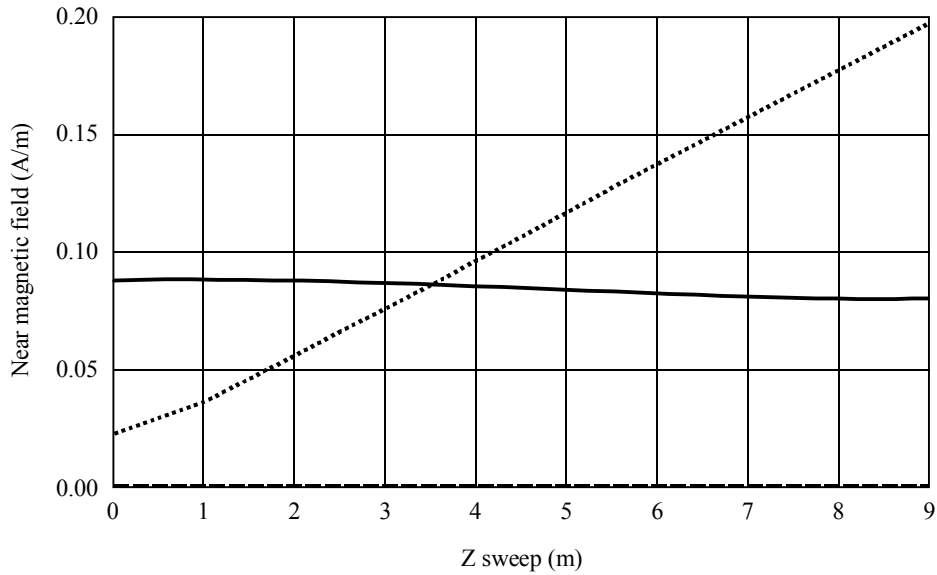

13 MHz, near magnetic field versus height @ 60 m from antenna.
 Transmitter power: 225 kW at antenna connector.

- Near magnetic field, mag (X), Z sweep, constants: X = 0, Y = 60; CORT13
- Near magnetic field, mag (Y), Z sweep, constants: X = 0, Y = 60; CORT13
- Near magnetic field, mag (Z), Z sweep, constants: X = 0, Y = 60; CORT13

Rap 2037-30


It is evident the strong relationship between H values and height (both z and y components of H field are present, y component's value is quite constant).

2.1.2 Measurements

Measurements have been performed using a broadband field strength meter installed over a dielectric trolley moved by an operator placed far away from the antenna site. In this way any kind of perturbation on E/H field is avoided.


2.1.2.1 Results of measurements

Measured values are presented in Fig. 31 (E field) and Fig. 32 (H field). Fig. 31 and Fig. 32 are directly comparable with Fig. 27 and Fig. 28 respectively.

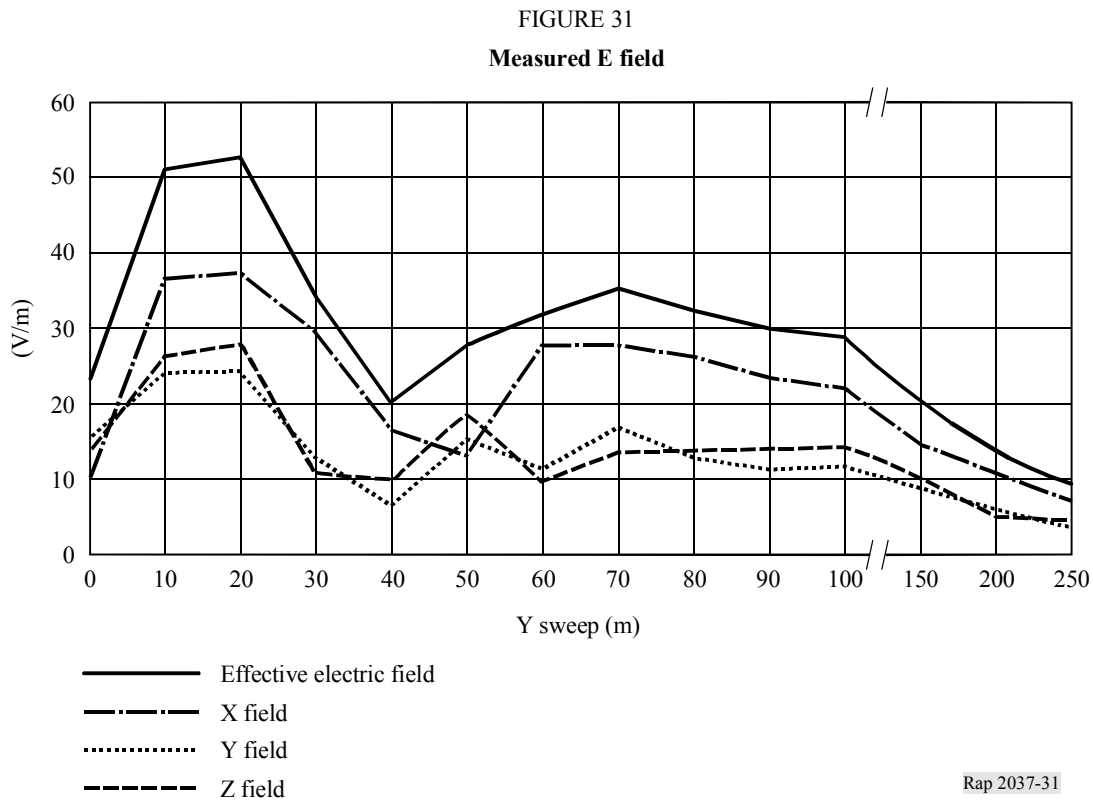

On the horizontal axis is represented the distance in metres from antenna (Y sweep). The intensity of E field's components is represented in V/m on vertical axis. All the three components x, y, z of E field are present, and the upper line represents the global value.

FIGURE 32
Measured H field

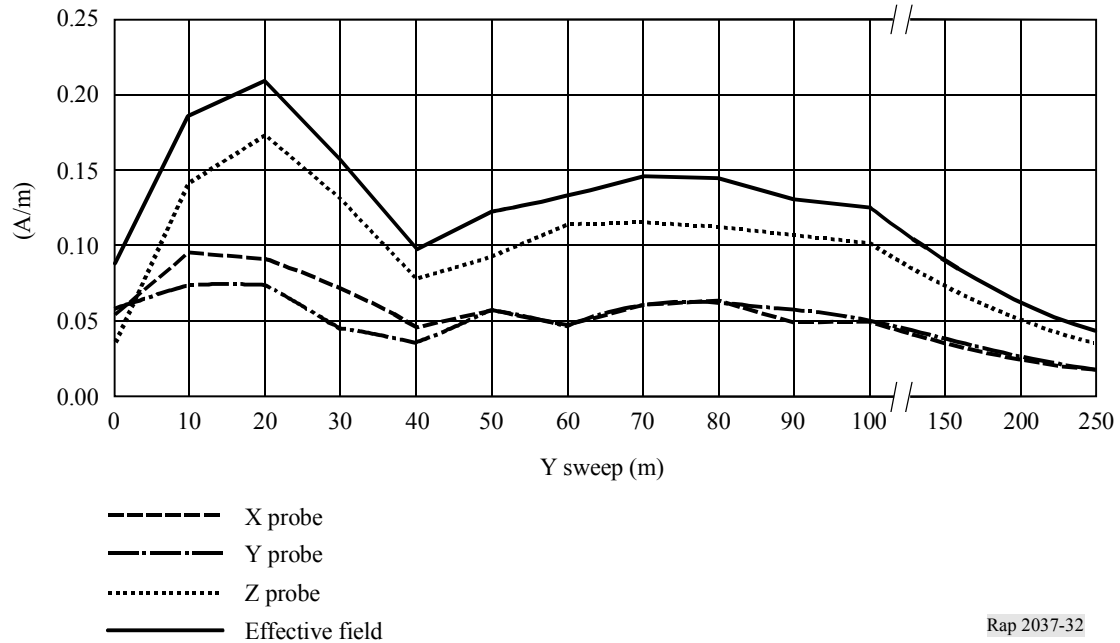

Rap 2037-32

On the horizontal axis is represented the distance in metres from antenna (Y sweep). The intensity of H field's components is represented in A/m on vertical axis. All the three components x, y, z of H field are present, and the upper line represents the global value.

2.2 18 MHz


2.2.1 Predictions

2.2.1.1 Notes about the model

In order to best fit the previously described model to the real antenna system, it is necessary to know the right amount of power at the input of each dipole, taking into account losses in transmission line and losses due to mismatch.

In order to apply the appropriate voltage value at each dipole, in the simulation the input impedance of each dipole has been calculated. The values are represented in Fig. 33.

FIGURE 33

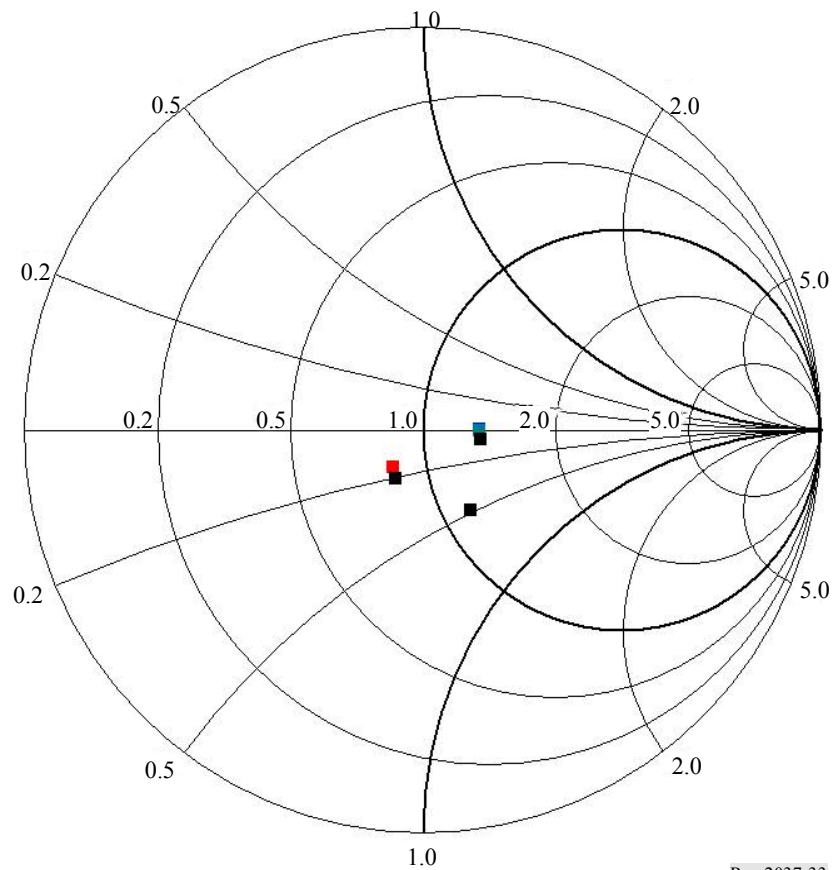Input impedance of dipoles, normalized to 180 Ω 18 MHz, dipoles impedance (normalized 180 Ω)

Rap 2037-33

Then, for each dipole has been adopted a common value of resistance equal to 180 Ω this being the average value obtained from the simulation. Note that this decision may be the cause of the inaccuracy in the prediction results.


Thanks to the low reactive components of input complex impedance, no adjustments of transmitter power have been necessary in order to compensate power losses due to the mismatch, and consequent reflection, between transmitter and antenna.

Note the little – but not inexistent – dispersion of resistance values near 180 Ω and the substantial absence of reactive components.

2.2.1.2 Far field evaluations


In order to best compare the behaviour of the model, with real antennas, given in Figs. 19 and 20 the radiation diagrams have been calculated. The results are shown in Fig. 34 (horizontal plane), Fig. 35 (vertical plane), Fig. 36 (frontal view).

FIGURE 34
Radiation diagram on horizontal plane

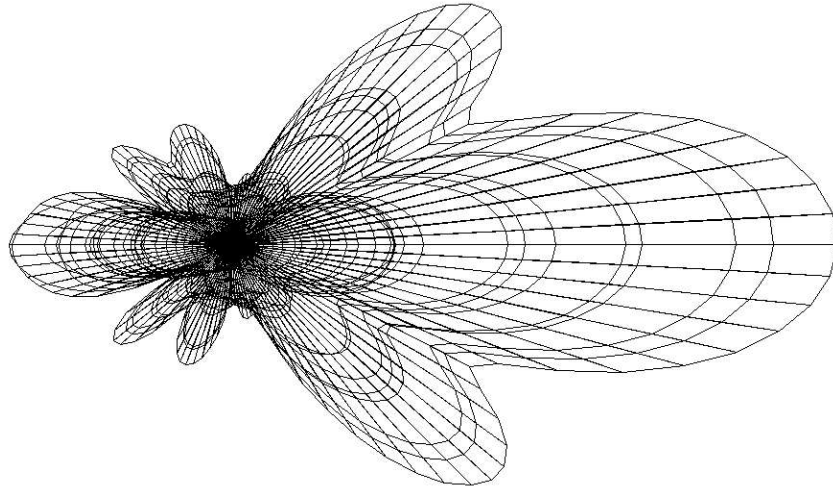


Rap 2037-34

FIGURE 35
Radiation diagram on vertical plane

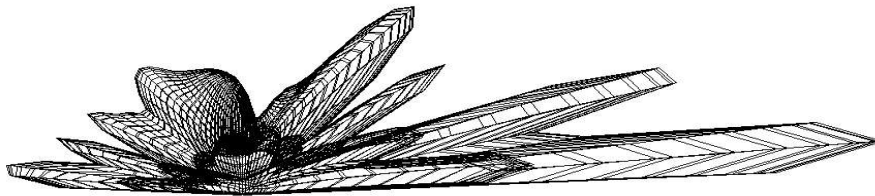

Rap 2037-35

FIGURE 36
Radiation diagram, front view

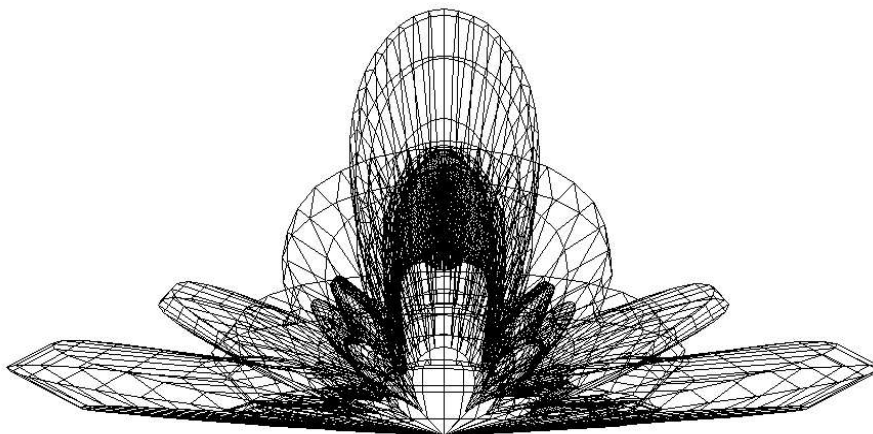


Rap 2037-36

2.2.1.3 Results of prediction of the field strength in the near zone

Prediction was made calculating the x, y, z components of E and H fields in the direction of the antenna's maximum gain (Y axis) at 2 m over terrain (Z axis = 2). The calculated values are represented in Fig. 37 (E field) and Fig. 38 (H field). The strong influence of the terrain both in the evaluations and in the measurements may introduce an additional difference between the two results. In order to show the strong influence of terrain, the E and H fields values have also been calculated varying the height of the evaluation point over the terrain (Z axis) from 0 up 9 m at a fixed distance of 60 m (Y = 60). The behaviour is illustrated in Fig. 39 (E field) and Fig. 40 (H field).

FIGURE 37
Calculated E field strength in the near zone

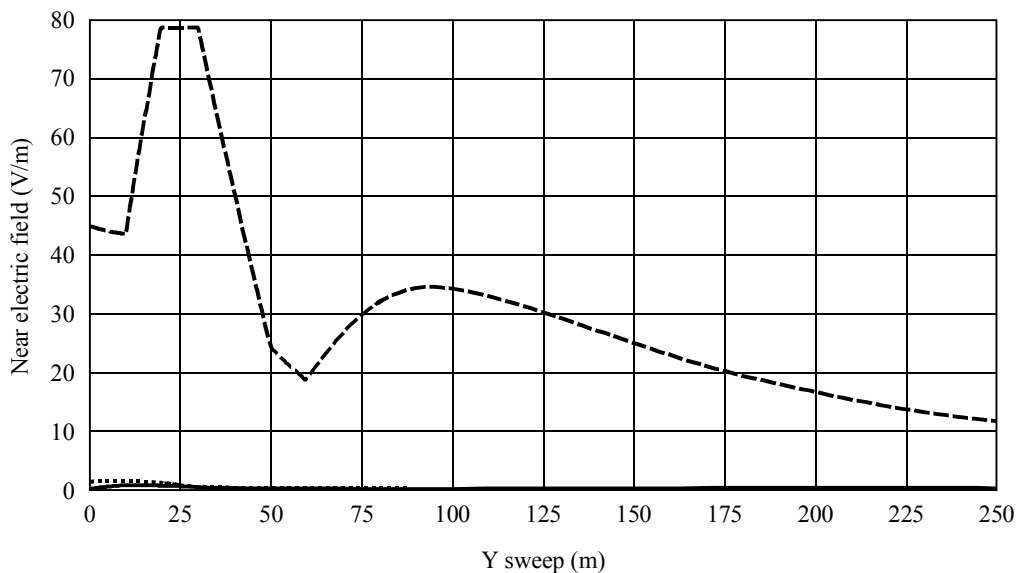


18 MHz, near electric field versus distance. Transmitter power: 200 kW at antenna connector.
Height: 2 m over terrain

- Near electric field, mag (X), Y sweep, constants: X = 0, Z = 2; CORT18
- Near electric field, mag (Y), Y sweep, constants: X = 0, Z = 2; CORT18
- Near electric field, mag (Z), Y sweep, constants: X = 0, Z = 2; CORT18

Rap 2037-37

The most important contribute is the x component. On the horizontal axis is represented the distance in metres from antenna (Y sweep). Z is fixed at 2 m (height over terrain). The intensity of E field's components is represented in V/m on vertical axis.

FIGURE 38
Calculated H field strength in the near zone

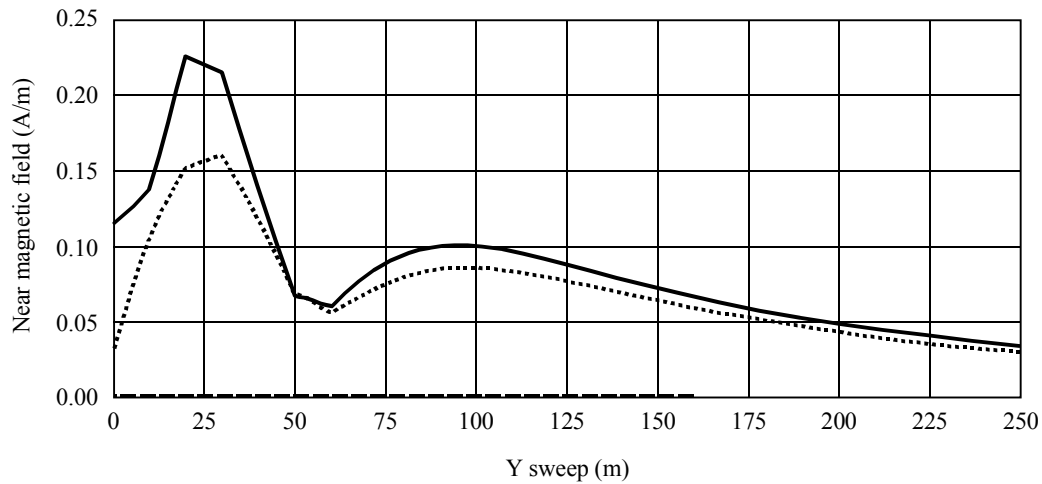


18 MHz, near magnetic field versus distance. Transmitter power: 200 kW at antenna connector. Height: 2 m over terrain

- Near magnetic field, mag (X), Y sweep, constants: X = 0, Z = 2; CORT18
- Near magnetic field, mag (Y), Y sweep, constants: X = 0, Z = 2; CORT18
- Near magnetic field, mag (Z), Y sweep, constants: X = 0, Z = 2; CORT18

Rap 2037-38

The main contribute is y component. The z component is lower, while x component is 0. On horizontal axis is represented the distance in metres from antenna (Y sweep). Z is fixed at 2 m (height over terrain). The intensity of H field's components is represented in A/m on vertical axis.

FIGURE 39
 Calculated E field strength at a distance of 60 m from antenna (Y = 60)
 at different heights between 0 and 9 m (Z sweep)

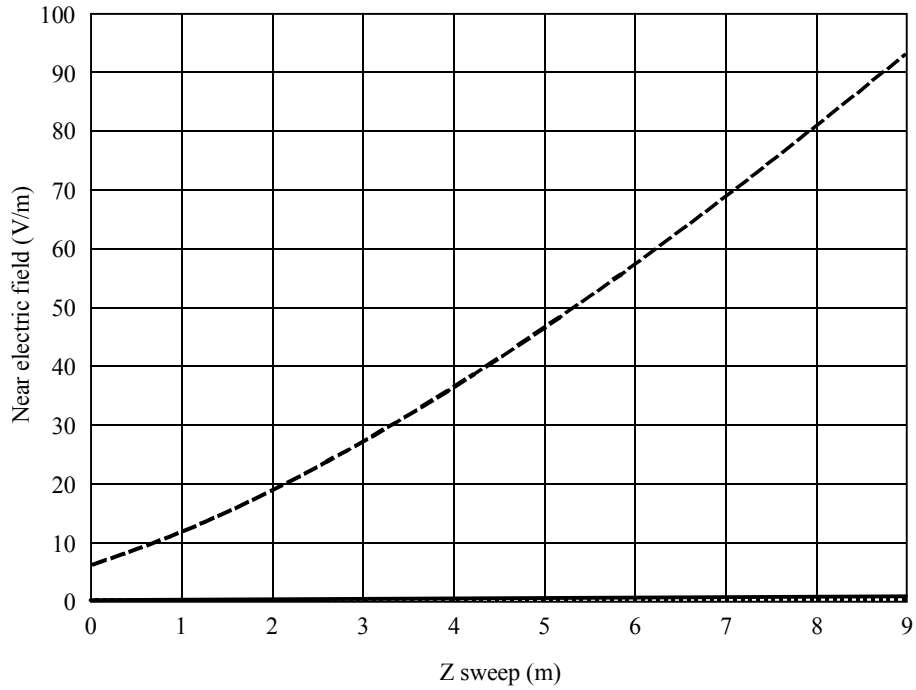

18 MHz, near electric field versus height @ 60 m from antenna.
 Transmitter power: 200 kW at antenna connector.


- Near electric field, mag (X), Z sweep, constants: X = 0, Y = 60; CORT18
- Near electric field, mag (Y), Z sweep, constants: X = 0, Y = 60; CORT18
- Near electric field, mag (Z), Z sweep, constants: X = 0, Y = 60; CORT18

Rap 2037-39

It is evident the strong relationship between E values and height (only x component of E field is present).

FIGURE 40

Calculated H field strength in the near zone at a distance of 60 m from antenna ($Y = 60$) at different heights between 0 and 9 m (Z sweep)

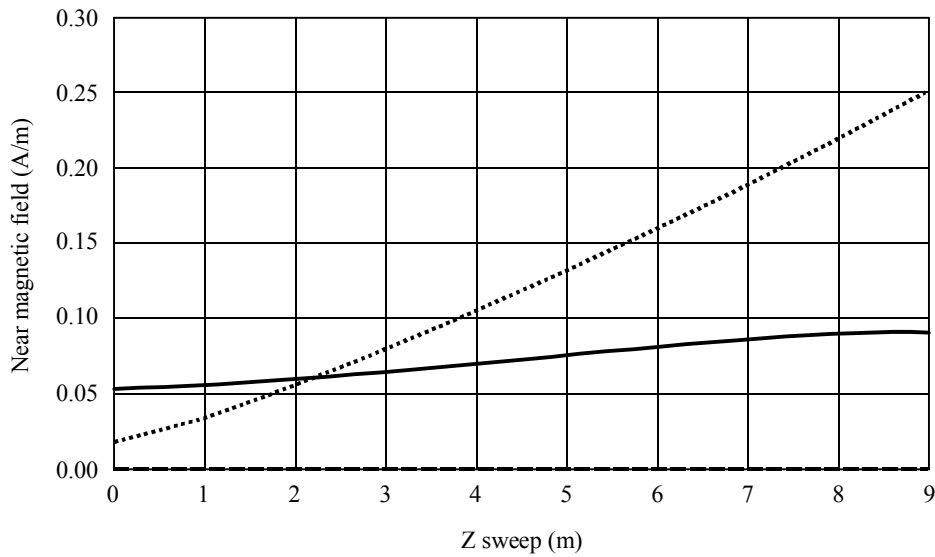

18 MHz, near magnetic field versus height @ 60 m from antenna.
Transmitter power: 200 kW at antenna connector.

- Near magnetic field, mag (X), Z sweep, constants: X = 0, Y = 60; CORT18
- Near magnetic field, mag (Y), Z sweep, constants: X = 0, Y = 60; CORT18
- Near magnetic field, mag (Z), Z sweep, constants: X = 0, Y = 60; CORT18

Rap 2037-40

It is evident the strong relationship between H values and height (both z and y components of H field are present, y component's value is quite constant).


2.2.2 Measurements

Measurements have been performed using a broadband field strength meter installed over a dielectric trolley moved by an operator placed far away from the antenna site. In this manner any kind of perturbation on the E/H field is avoided.

2.2.2.1 Results of measurements

Measured values are presented in Fig. 41 (E field) and Fig. 42 (H field). Figs. 41 and 42 are directly comparable with Figs. 37 and 38 respectively.

FIGURE 41
Measured E field strength in the near zone

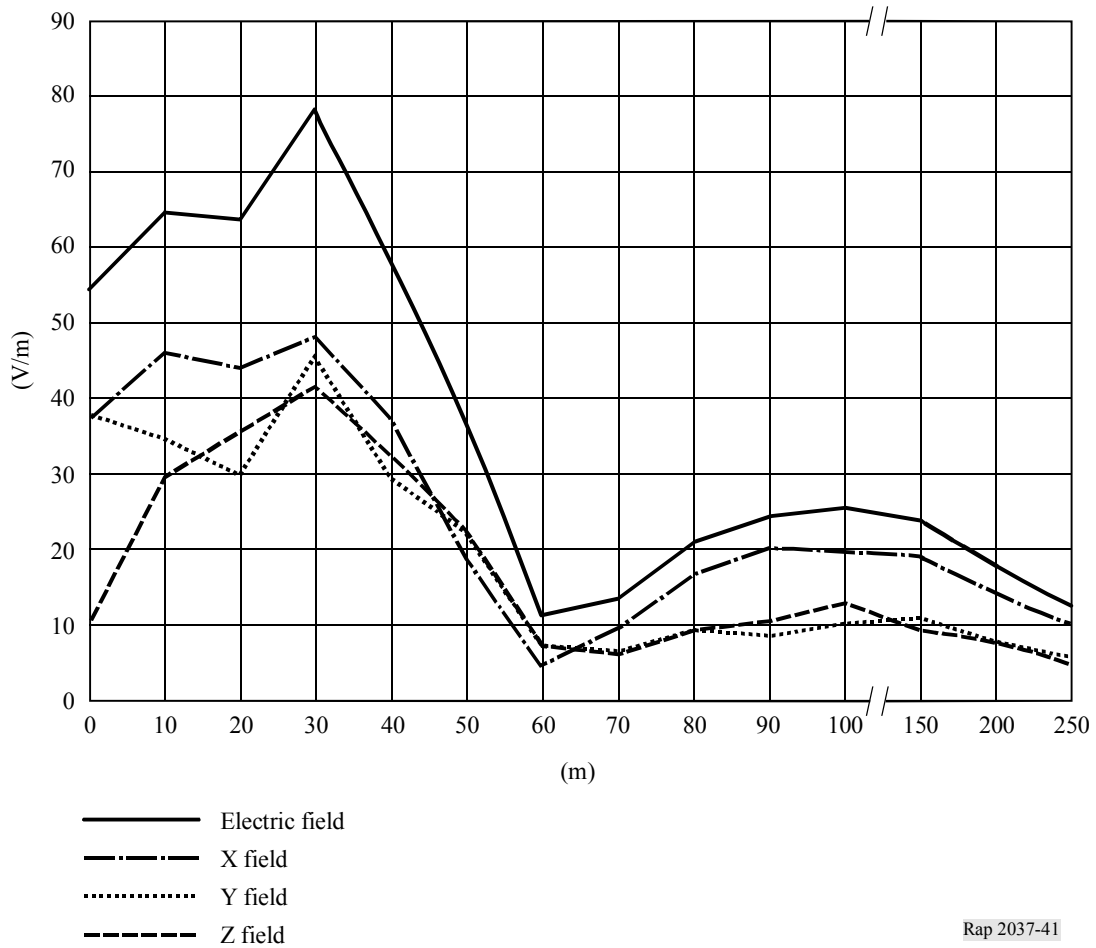


Rap 2037-41

On the horizontal axis is represented the distance in metres from antenna (Y sweep). The intensity of E field's components is represented in V/m on vertical axis. All the three components x, y, z of E field are present, and the upper line represents the global value.

FIGURE 42

Measured H field strength in the near zone

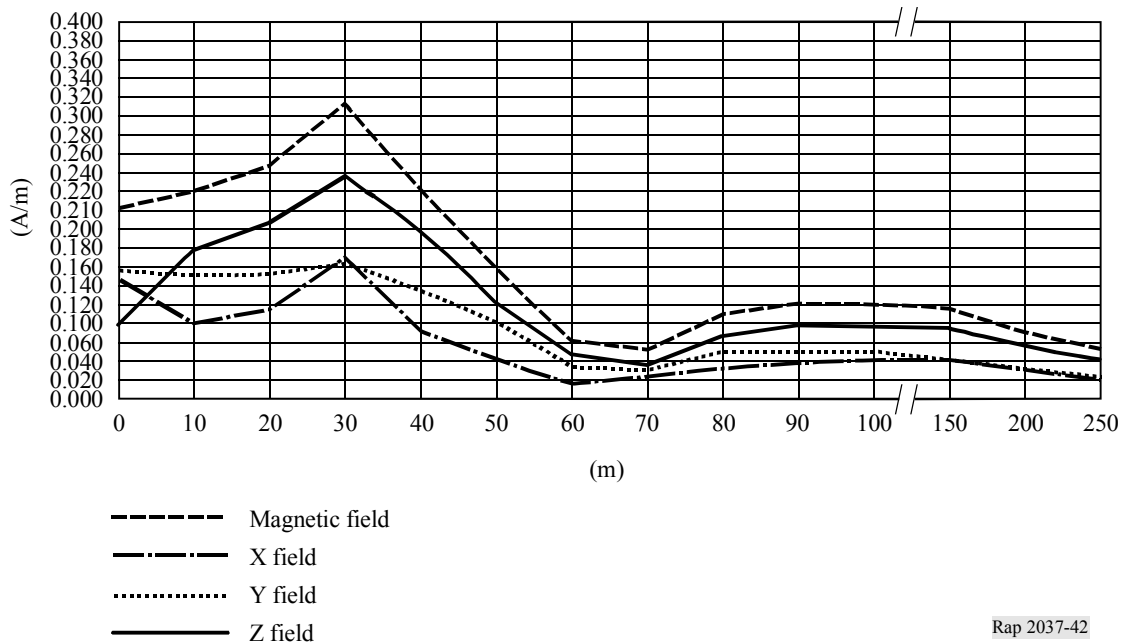

On the horizontal axis is represented the distance in metres from antenna (Y sweep). The intensity of H field's components is represented in A/m on vertical axis. All the three components x, y, z of H field are present, and the upper line.

2.3 Comparison between measurements and predictions of the field strength in the near zone

2.3.1 13 MHz

At a distance less than 40 m prediction has given values, of both E and H field, higher than measured ones; anyway, the maximum values of E and H were found at a distance of 10-20 m from the antenna system, in both the simulation results and in measurements.

Both in predicted and in measured values there is an evident "minimum" at 40 m from antenna, deeper in prediction than in measurement.

The second "maximum" reaches its peak, in both cases, at 75 m from antenna; in this case the values obtained from simulations are lower than the measured ones.

At a long distance, 250 m from the antenna, all the fields reach practically the same values between prediction and measurement.

2.3.2 18 MHz

At a distance less than 40 m prediction has given values, of both E and H field, higher than measured ones; anyway, the maximum values of E and H were found at a distance of 10-20 m from the antenna system, in both the simulation results and in measurements.

A second “maximum” is reached at 100 m, both in prediction and in measurement for E and H field, with a lower value for measured E field. At a distance higher than 60 m from the antenna H field assumes the same value both in prediction and in measurement.

3 Conclusions

The comparison between measured and predicted values of E and H fields both at 13 MHz and 18 MHz gives interesting results.

Values are, generally, not properly coincident, as seems obvious to expect; however there are not substantial differences among them, if compared with uncertainty of instrumentation, uncertainty in planarity of heart's surface near antenna (not taken into account in simulations even if it is clear the strong dependence of fields intensity by height of measurement point) and the imposed simplicity of the model. Differences are bigger near the antenna (i.e. the first maximum at about 10 m), up to 50%, and decrease with the distance; at 250 m the differences are quite zero.

The reasons for these differences are to be searched in the difficulties in near field measurements, the uncertainty inherent the instrumentation, the simplicity of the model, the presence of some objects near the antenna (metallic structures, the two lattices supporting dipoles and matching network, a little house) that has not taken into account in the model, as well as the matching network and its radiation. Finally, terrain has been modelled with its typical electrical values.

In order to best approach the activity of E/H field's prediction by a simulator, we remark some notes:

Antenna model: physical dimension of radiating and passive elements are to be carefully investigated as well as the complex input impedance of the system. In order to simplify a complex system, i.e. an array of radiators, it may be convenient to substitute the matching and feeding network with an equal number of voltage generators applied at the input of each radiator. If the matching network is not considered, then it is necessary to compensate the:

- Eventual mismatch between generators and radiators by the introduction of artificial matching elements or simple networks, or adjusting the power assigned to the transmitter. The final result is quite insensitive to the presence of little mismatches that is generally not necessary to compensate.

Segment subdivision: it is sufficient to represent filar antenna systems with segments not longer than $\lambda/20$.

Terrain model: it is necessary to give the exact values of permittivity and conductivity, especially in case of horizontally-polarized E field.

Transmitter power: it is important to take into account losses in transmission lines, matching network, resistance of junctions, mismatches to the load. In some cases it is opportune to artificially adjust the exact value of power in order to take into account various causes of losses without complicating the model of the antenna system.

Height of measurement points referred to ground: in many cases this parameter is very important if the scope is a comparison between measurements and predictions. In fact a strong influence of height may be noted in the value of fields, and, if the terrain is modelled as a plain, big mistakes may be encountered in the comparison with a measurement. In all these cases in which radiators are in vicinity of terrain and terrain is not quite plane, the results of prediction must be taken with prudence.

Selection of code: the simulation based on MOM seems to be useful and easy to use in cases of filar antennas of which are well known physical and electrical characteristics. It is possible and quite easy to simplify the model according to a minimum number of rules, without loss in precision of results.

Appendix 3

Limits and levels

1 Regulatory and advisory authorities on health aspects

A number of international and national authorities are concerned with the health aspects of EMFs. This non-exhaustive list is given at the end of this Appendix for information.

2 Comparison of basic limits and derived levels from widely used regulations

Present standard guidelines differ in the definition of groups of persons potentially at risk “exposure groups” (e.g. general public, occupationally exposed workers, age) and/or in the place of locations of interest (e.g. public places, houses, fenced enclosures and restricted buildings).

Differences also appear on the parts of the body considered.

In this Appendix are compared:

- IEEE Standard for safety levels with respect to human exposure to radio frequency electromagnetic fields, 3 kHz to 300 GHz [3].
- Guidelines for limiting of exposure to time-varying electric, magnetic and electromagnetic fields (up to 300 GHz) [4].
- Board statement on restrictions on human exposure to static and time varying electromagnetic fields and radiation [5].

Table 5 gives an approximate comparison between groups and locations selected in the standards.

TABLE 5

	IEEE/ANSI	ICNIRP	NRPB
Groups	No	General public Occupationally exposed people	Adults and children Adults
Locations	Controlled (Awareness of exposed people) Uncontrolled (No awareness)	No	No

2.1 Comparison of basic biological limits

Standards and guidelines give “basic limits” for contact current, current density and SAR and are reported in Table 6, together with measuring conditions.

A common guideline for compared standards is that all of them do not allow SAR over the entire body to exceed the value of 4 W/kg.

By applying a safety factor of 10, basic SAR limit (whole-body-averaged SAR) is reduced to 0.4 W/kg. The NRPB basic limit of 0.4 W/kg is proposed as the maximum level allowed for core temperature increase of 1 K.

It is to be noted that the basic whole body limit for SAR is averaged over a time of 6 min. There are also limits applicable to specific part of the body, referred as “local SARs”; since resonance effects may give rise to local “hot spots”, these limits are higher than the whole-body-averaged SAR.

2.2 Comparison of derived limit levels for E, H and power flux limits at various frequencies

The direct measurement of the current density and specific absorption rate is very difficult and not possible in practice. Therefore, derived levels are given in addition to the basic limits, in the standards and guidelines considered here.

On the other hand measurement of EM field quantities E and H are of more practical feasibility.

SAR is frequency dependent, while the basic limits as in Table 6 are assumed constant. By means of the relevant the SAR limit may be transformed into free field corresponding quantities E,H,S.

TABLE 6

Comparison of basic biological restrictions (SAR limits) and reference levels (current parameters)

Parameter	IEEE/ANSI		ICNIRP		NRPB
	Controlled	Uncontrolled	Occupational	General Public	
RMS induced or contact current (mA)	$1\,000f$ (13a)	$450f$ (13a)	100 (2)	45 (2)	
	100 (1), (13b)	45 (1), (13b)	40 (3)	20 (3)	
Current density RMS (A/m ²) Averaging area (cm ²) Averaging times	$350f$ 1 1 (4)	$15.7f$ 1 1 (4)	$10f$ 1 (4)	$2f$ 1 (4)	$10f$
Whole-body-average (W/kg) SAR	0.4 (5a)	0.08 (5b)	0.4 (5a)	0.08 (5a)	0.4 (5c)
Local SAR (W/kg) Averaging mass (kg)	8 (13c) 0.001 (6)	1.6 (13c) 0.001 (6)	10 (13d) 0.001 (5a), (7)	2 (13d) 0.01 (5a), (7)	10 0.01 and 0.1 (N.11) (5a), (10)
Local SAR ⁽⁷⁾ (W/kg) Averaging mass (kg)	20 (13c) 0.010 ⁽⁸⁾	4 (13c) 0.010 ⁽⁸⁾	20 (13d) 0.001 ^{(5a), (9)}	4 (13d) 0.01 ^{(5a), (9)}	20 0.1 ^{(5a), (9)}
Power density (W/m ²) Averaging time (min)			50 $68/f^{1.05}$ (12), (13)	10 $68/f^{1.05}$ (12), (13)	100 $68/f^{1.05}$ (12)

f : frequency in MHz (unless otherwise stated).

- (1) Current through each foot. f : frequency (MHz).
(2) Current induced in any limb (10-110 MHz).
(3) Contact current from conductive objects (100 kHz-110 MHz).
(4) Current density over any 1 cm² area of tissue
(5) a) The SAR limits relate to an averaging time of 6 min.
b) The SAR limits relate to an averaging time as given in Table 7.
c) The SAR limits relate to an averaging time of 15 min.
(6) Localized SAR except for the hands, wrists, feet and ankles (100 kHz-6 GHz).
(7) Localized SAR for head and trunk (100 kHz-10 GHz)
(8) Localized SAR for the hands, wrists, feet and ankles (100 kHz-6 GHz).
(9) Localized SAR for limbs (100 kHz-10 GHz).
(10) Localized SAR for head, neck, trunk and foetus (10 MHz-10 GHz).
(11) 10 g for the head and foetus; 100 g for the neck and trunk.
(12) For frequencies between 10 and 300 GHz. f : frequency (GHz).
(13) Averaged over any 20 cm² of exposed area:
a) 3 kHz < f < 100 kHz
b) 100 kHz < f < 100 MHz
c) 100 kHz < f < 6 GHz
d) 100 kHz < f < 10 GHz.

Tables 7, 8 and 9 show the maximum level respectively of E, H, and pfd in various bands in the frequency range 1 kHz-300 GHz. The limits are calculated under the conservative assumption of optimum electromagnetic coupling between the EMF and the body.

TABLE 7

Comparison of derived levels; E field (r.m.s. values V/m)*

Frequency range	IEEE/ANSI		ICNIRP		NRPB							
	Controlled	Uncontrolled	Occupational	General public	Adults only	Adults and children						
0.6-3 kHz					1 000							
3-30 kHz	614		610 ⁽¹⁾	87								
30-38 kHz												
38-65 kHz												
65-100 kHz												
100-410 kHz												
410-600 kHz												
600-610 kHz												
610-680 kHz												
680-920 kHz												
0.92-1 MHz												
1-1.34 MHz	614		610/ <i>f</i>	87/ <i>f</i> ^{0.5}	600/ <i>f</i>							
1.34-3 MHz												
3-10 MHz	1 842/ <i>f</i>		61	28	60	600/ <i>f</i>						
10-12 MHz	823.8/ <i>f</i>											
12-30 MHz	61.4				27.5	<i>f</i> ⁽²⁾	50 ⁽²⁾					
30-60 MHz												
60-100 MHz												
100-137 MHz												
137-200 MHz												
200-300 MHz					3 <i>f</i> ^{0.5}	1.375 <i>f</i> ^{0.5}	137 ⁽²⁾	0.25 <i>f</i> ⁽²⁾				
300-400 MHz												
400-800 MHz											100 ⁽²⁾	
0.8-1.1 GHz												
1.1-1.55 GHz					0.125 <i>f</i> ⁽²⁾	0.125 <i>f</i> ⁽²⁾						
1.55-2 GHz												
2-3 GHz									137	61	194 ⁽²⁾	
3-15 GHz												
15-300 GHz												

f: frequency (MHz, unless otherwise stated).

* Values should be averaged over 6 min, except as shown below:

- a) $f^2/0.3$
- b) 30 min.

⁽¹⁾ This value is in the range 0.82 kHz to 1 MHz.

⁽²⁾ Plane wave equivalent value of the E field.

TABLE 8
Comparison of derived levels; H field (RMS values A/m)^{(1), (2)}

Frequency range	IEEE/ANSI		ICNIRP		NRPB			
	Controlled	Uncontrolled	Occupational	General public	Adults only	Adults and children		
1-3 kHz					64			
3-30 kHz	163							
30-38 kHz								
38-65 kHz								
65-100 kHz								
100-140 kHz			5 ⁽³⁾					
140-150 kHz	16.3/f		1.6/f				18/f ²	
150-535 kHz								
535-610 kHz								
610-680 kHz								
0.68-1 MHz				0.73/f				
1-1.34 MHz								
1.34-3 MHz								
3-10 MHz								
10-12 MHz								
12-30 MHz								
30-60 MHz	16.3/f	158.3/f ^{1.668} (1a))						
60-100 MHz			0.16	0.073	f/377 ⁽²⁾	0.13		
100-137 MHz	0.163							
137-200 MHz								
200-300 MHz			0.0729					
300-400 MHz			(1b))			0.36 ⁽²⁾	0.66 × 10 ⁻³ f	
400-800 MHz							0.26	
0.8-1.1 GHz			0.008f ^{0.5}	0.0037f ^{0.5}		0.33 × 10 ⁻³ f		
1.1-1.55 GHz					0.33 × 10 ⁻³ f ⁽²⁾			
1.55-2 GHz					0.52			
2-3 GHz								
3-15 GHz			0.36	0.16				
15-300 GHz								

f : frequency (MHz, unless otherwise stated).

(1) Values should be averaged over 6 min, except as shown below:

- a) $0.0636 f^{1.337}$ min
- b) 30 min.

(2) Plane wave equivalent value of the H field, based on power density values given for adults. NOTE – These values are not given explicitly in the same way as the E field and power density values are specified.

(3) This value is valid in the range 0.8 kHz to 150 kHz.

TABLE 9

Comparison of derived levels; pfd (W/m^2)^{(1), (4)}

Frequency range	IEEE/ANSI ⁽²⁾				ICNIRP		NRPB	
	Controlled		Uncontrolled		Occupational	General public	Adults only	Adults and children
	E field	H field	E field	H field				
<100 Hz								
0.1-1 kHz								
1-3 kHz								
3-30 kHz								
30-100 kHz	1 000	10×10^6	1 000	10×10^6				
100-410 kHz								
0.41-1 MHz	1 000	$10^5 f^2$	1 000	$10^5 f^2$				
1-1.34 MHz								
1.34-3 MHz	1 000	$10^5 f^2$	$1\,800/f^2$ (3), (4a))	$10^5 f^2$ (3)				
3-10 MHz								
10-12 MHz	$9\,000/f^2$	$10^5 f^2$	$1\,800/f^2$ (3), (4b))	$10^5 f^2$ (3)	10	2	10	6.6
12-30 MHz								
30-60 MHz			2 (3), (4b))	$(9.4 \times 10^6)/f^{8.336}$ (3), (4c))				
60-100 MHz	10	$10^5 f^2$					$2.7 \times 10^{-3} f^2$	
100-137 MHz								
137-200 MHz	10		2 (4b))					
200-300 MHz								$0.165 \times 10^{-3} f^2$
300-400 MHz							50	
400-800 MHz								26
0.8-1.1 GHz			$f/150$					$41 \times 10^{-6} f^2$
1.1-1.55 GHz	$f/30$				$f/40$	$f/200$	$41 \times 10^{-6} f^2$	
1.55-2 GHz			(4b))					
2-3 GHz							100	
3-15 GHz	100		$f/150$ (4d))		50	10		
15-300 GHz	100 ^(4e)							

⁽¹⁾ f : frequency (MHz, unless otherwise stated).

⁽²⁾ Below 100 MHz, plane-wave equivalent values are given for the E and H fields.

⁽³⁾ As given by some commercially available metres.

⁽⁴⁾ Values should be averaged over 6 min, except as shown below:

- a) $f^2/0.3$ min
- b) 30 min
- c) $0.0336 f^{1.337}$ min
- d) $90\,000/f$ min
- e) $616\,000/f^{1.2}$ min.

3 Field-strength values to be determined


Preliminary, using data given in the tables in this Appendix, § 3.2 the range of electrical and magnetic field strengths are shown in Figs. 43 and 44, respectively.

These curves/graphs should not be used as a basis for an administration's regulatory requirements. They represent a composite view of the limits currently depicted and are certain to evolve over time. As such, they are merely illustrative of the methodology that could be applied to develop useful standards within an administration.

Also, it must be recognized that results of independent studies of the subject are not entirely consistent and as a result the interpretation of the results by responsible authorities has in the past and will continue in the future to result in differing requirements in different countries.

FIGURE 43


The range of the electrical field strengths derived from the tables given in Appendix 3

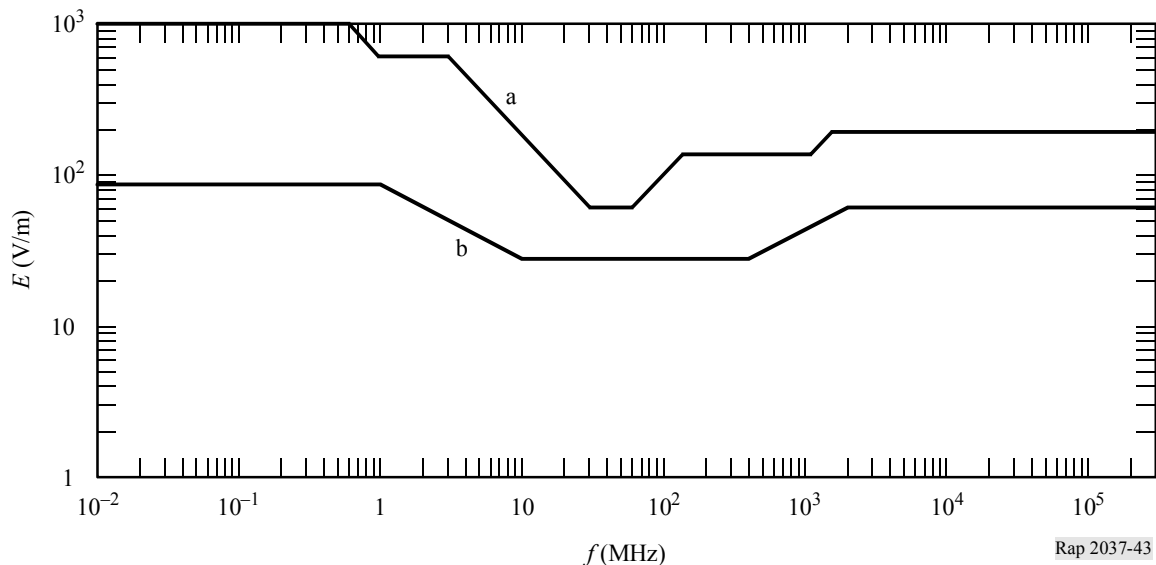

The curves “a” and “b” represent the upper and lower boundaries respectively of some known, existing recommendations for RF exposures levels (presented in this Appendix, as example). All curves from authorities making such recommendation lie between these boundaries, and any curve between curves “a” and “b” should allow adequate broadcasting services.

FIGURE 44

The range of the magnetic field strengths derived from the tables given in this Appendix

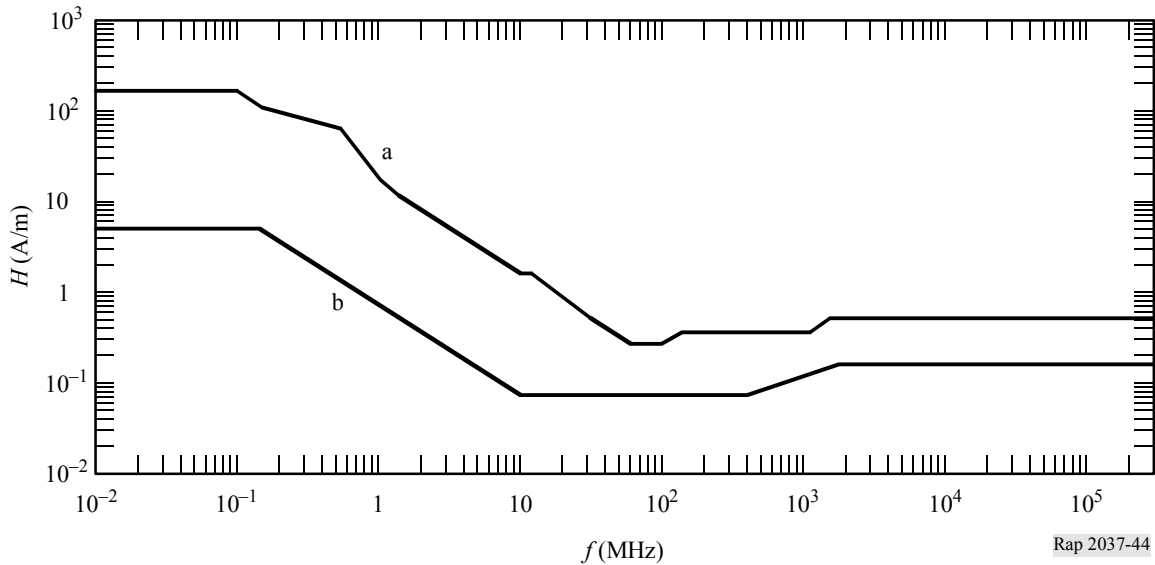

The curves “a” and “b” represent the upper and lower boundaries respectively of some known, existing recommendations for RF exposures levels (presented in this Appendix, as example). All curves from authorities making such recommendation lie between these boundaries, and any curve between curves “a” and “b” should allow adequate broadcasting services.

The differences between the suggested maximum levels at the same frequency (Figs. 43 and 44) depend on different conditions considered by the various sources suggesting the limits.

4 Numerical procedures and calculation of EMF quantities

In few relatively simple cases, electromagnetic radiation and scatter problems can be solved by using analytic procedures in a closed form. However, the solution of general problems, with random geometries, requires the application of numerical calculation procedures, running on powerful computers.

The numerical procedures, depending on the frequency range under consideration and the size of the geometrical structures used, are available for the calculation of EMF field quantities.

Among these different methods we have decided to use the MOM, used in the design of broadcast antenna systems and in calculating their resultant electromagnetic fields.

The MOM is used intensively for calculating the SAR distribution in so-called /block model/.

The electric field intensities within the body are calculated from the solution of the integral equation of the electric field by using Maxwell’s equations.

The software used is: NEC – WIN Professional V 1.1 (1997) by Nittany Scientific, inc. – www.nittany-scientific.com.

5 List of some national regulations

5.1 Administrations

5.1.1 Australia

Australian Radiation Protection and Nuclear Safety Agency (ARPANSA) Radiation Protection Standard RPS-3, Radiation Protection Standard – Maximum exposure levels to radiofrequency fields – 3 kHz to 300 GHz.

5.1.2 Brazil

Resolution n. 303/202 – Regulamento sobre Limitacao da Exposicao a Campos Elétricos, Magnéticos e Elétromagnéticos na Faixa de Radiofrecuencias entre 9 kHz e 300 GHz. www.anatel.gov.br/biblioteca/Templates/Resolucoes/resolucoes.asp.

5.1.3 France

Decree nb.2002-775 of 03.05.2002, relating to the limit values of public exposure o the electromagnetic fields radiated by the equipment used in the telecommunication networks or by the radioelectric installations.

5.1.4 Germany

Bundesministeriu fuer Wirtschaft und Arbeit www.bmwi.de.

5.1.5 Italy

DPCM 8 July 2003. www.parlamento.it/parlam/leggi/elelenum.htm.

5.1.6 New Zealand

5.1.7 United States of America

<http://www.fcc.gov/oet/rfsafety/>.

5.1.8 Vatican City State

Delibera del 16/12/1992 No: 225620.

5.1.9 Japan

Radio Law (Law No. 131 of May 2, 1950), Article 30.

The Regulations for Enforcement of the Radio Law (Radio Regulatory Commission Rules No. 14 of November 30, 1950), Article 21-3 and Annex Table 2-3-2.

Website: <http://www.tele.soumu.go.jp/e/ele/index.htm> (in English)

<http://www.tele.soumu.go.jp/j/ele/index.htm> (in Japanese)

(The Articles of the Law and the Regulations are available only in Japanese. Some reports to the Ministry are available in English.)

- 6 List of some Regulatory and Advisory bodies**
- 6.1 Electronic Components Committee, Comité des composants électroniques, CENELEC [4]**
- 6.2 German Commission for Electrical and Electronic Information technologies, DKE**
- 6.3 European Union, EU – “Recommendation from the Council of the European Union” L 199, 12 July 1999**
- 6.4 Institute of Electrical and Electronics Engineer/ American National Standards Institute, IEEE/ANSI**
- 6.5 International Commission on non-ionizing radiation, ICNIRP**
- 6.6 International Electrotechnical Commission, IEC**
- 6.7 World Health Organization, WHO**
- 6.8 National Radiological Protection Board, NRPB**
- 6.9 European Telecommunications Standards Institute, ETSI**

Appendix 4

Additional evaluation methods

1 Dosimetry

The application of dosimetric concepts enables the link to be established between external (i.e. outside the body) field strengths and internal quantities of electric field strength, induced current density and the energy absorption rate in tissues. The development of experimental and numerical dosimetry has been complementary. Both approaches necessitate approximations to the simulation of human exposure; however the development of tissue equivalent materials and minimally disturbing probes in the experimental domain and the use of anatomically realistic models for computational purposes has improved the understanding of the interaction of RF fields with the body.

Whereas current density is the quantity most clearly related to the biological effects at low frequencies, it is the SAR, which becomes the more significant quantity as frequencies increase towards wavelengths comparable to the human body dimensions.

In most exposure situations the SAR can only be inferred from measured field strengths in the environment using dosimetric models. At frequencies below 100 MHz non-invasive techniques have been used to measure induced current, and in extended uniform fields, external electric field strengths have been related to induced current as a function of frequency. In the body resonance region, exposures of practical significance arise in the reactive near field where coupling of the incident field with the body is difficult to establish owing to non-uniformity of the field and changing alignment between field and body. In addition, localized increases in current density and SAR may arise in parts of the body as a consequence of the restricted geometrical cross-section of the more conductive tissues.

Dosimetric quantities can be calculated by use of suitable numeric procedures and calculational models of the human body. On the other hand such quantities can be measured using suitable physical models (phantoms).

2 SAR measurement

The SAR (W/kg), is the basic limit quantity of most RF exposure regulations and standards. SAR is a measure of the rate of electromagnetic energy dissipated per unit mass of tissue.

The SAR may be specified as the value normalized over the whole body mass (sometimes referred to as the “whole body averaged SAR”) or the localized value over a small volume of tissue (localized SAR).

SAR can be ascertained from the internal quantities in three ways, as indicated by the following equation:

$$SAR = \frac{\sigma E^2}{\rho} = C_i \frac{dT}{dt} = \frac{J^2}{\sigma \rho}$$

where:

E : value of the internal electric field strength in the body tissue (V/m^{-1})

σ : conductivity of body tissue (S/m^{-1})

ρ : density of body tissue (kg/m^{-3})

C_i : heat capacity of body tissue ($J/kg^{-1} \text{ } ^\circ C^{-1}$)

dT/dt : time derivative of temperature in body tissue ($^\circ C/s^{-1}$)

J : value of the induced current density in the body tissue (A/m^2).

The local SAR in an incremental mass (dm) is defined as the time derivative of the incremental absorbed energy (dW) divided by the mass:

$$SAR = \frac{dW}{dm \, dt}$$

This quantity value is important from two standpoints; the resulting non-uniform distribution of energy absorption when exposed to a uniform plane wave, and the localized energy absorption arising from non-uniform fields in close proximity to a source of exposure.

Exposure regulations or standards contain derived electric and magnetic field limits. The underlying dosimetric concept assures that compliance with the (external) derived levels will assure compliance with the basic SAR limits. However, external or internal SAR measurements can also be used to show compliance. For partial-body near-field exposure conditions, the external electromagnetic fields may be difficult to measure, or may exceed the derived limits although the local SAR is below the basic limits. In these cases internal SAR measurements in body models have to be conducted. The most important methods to measure SAR will be described below.

2.1 Electric field measurement

The SAR is also proportional to the squared RMS electric field strength E (V/m) inside the exposed tissue:

$$SAR = \sigma E^2 / \rho$$

where:

σ (S/m): conductivity

ρ (kg/m³): mass density of the tissue material at the position of interest.

Using an isotropic electric field probe, the local SAR inside an irradiated body model can be determined. By moving the probe and repeating the electric field measurements in the whole body or in a part of the body, the SAR distribution and the whole body or partial-body averaged SAR values can be determined. A single electric field measurement takes only a few seconds, which means that three-dimensional SAR distributions can be determined with high spatial resolution and with a reasonable measurement time (typically less than an hour).

2.2 Temperature measurement

The SAR is proportional to initial rate of temperature rise dT/dt (C/s) in the tissue of an exposed object:

$$SAR = c \Delta T / \Delta t$$

where c is the specific heat capacity of the tissue material (J/kgC). Using certain temperature probes, the local SAR inside an irradiated body model can be determined. One or more probes are used to determine the temperature rise ΔT during a short exposure time Δt (typically less than 30 s to prevent heat transfer). The initial rate of temperature rise is approximated by $\Delta T / \Delta t$, and the local SAR value is calculated for each measurement position. By repeating the temperature measurements in the whole body or in a part of the body, the SAR distribution and the whole-body or partial-body averaged SAR values can be determined.

Three-dimensional SAR-distribution measurements are very time consuming due to the large number of measurement points. To achieve a reasonable measurement time the number of points has to be limited. This means that it is very difficult to measure strongly non-uniform SAR distributions accurately. The accuracy of temperature measurements may also be affected by thermal conduction and convection during measurements, or between measurements.

2.3 Calorimetric measurement

The whole-body average SAR can be determined using calorimetric methods. In a normal calorimetric measurement, a full-size or scaled body model at thermal equilibrium is irradiated for a period of time. A calorimeter is then used to measure the heat flow from the body, until the model is at thermal equilibrium again. The obtained total absorbed energy is then divided by the exposure time and the mass of the body model, which gives the whole-body SAR. The calorimetric twin-well technique uses two calorimeters and two identical body models. One of the models is irradiated, and the other one is used as a thermal reference. This means that the measurement can be performed under less well-controlled thermal conditions than a normal calorimetric measurement.

Calorimetric measurements give rather accurate determinations of whole-body SAR, but do not give any information about the internal SAR distribution. To get accurate results a sufficient amount of energy deposition is required. The total time of a measurement, which is determined by the time to reach thermal equilibrium after exposure, may be up to several hours. Partial body SAR can be measured by using partial-body phantoms and small calorimeters.

3 Body current measurement

Measurement devices for body current may be carried out in two categories:

- measurement devices for body to ground current;
- measurement devices for contact current.

3.1 Induced body currents

Internal body currents are induced in persons occur from partial or whole-body exposure of the body to RF fields in the absence of contact with objects other than the ground.

The two principal techniques used for measuring body currents include clamp-on type (solenoidal) current transformers for measuring current flowing in the limbs, and parallel plate systems that permit the measurement of currents flowing to ground through the feet.

Clamp-on current transformer instruments have been developed that can be worn.

The meter unit is mounted either directly on the transformer or connected through a fibre-optic link to provide a display of the current flowing in a limb around which the current transformer is clamped. Current sensing in these units may be accomplished using either narrow-band techniques, e.g., spectrum analysers or tuned receivers (which offer the advantage of being able to determine the frequency distribution of the induced current in multi-source environments, or broadband techniques using diode detection or thermal conversion.

Instruments have been designed to provide true r.m.s. indications in the presence of multiple frequencies and/or amplitude-modulated waveforms.

The upper frequency response of current transformers is usually limited to about 100 MHz however air cored transformers (as opposed to ferrite-cored), have been used to extend the upper frequency response of these instruments. Whilst air-cored transformers are lighter and therefore useful for longer term measurements, they are significantly less sensitive than ferrite cored devices.

An alternative to the clamp-on device is the parallel plate system. In this instrument, the body current flows through the feet to a conductive top plate, through some form of current sensor mounted between the plates, and thereby to ground. The current flowing between the top and bottom plates may be determined by measuring the RF voltage drop across a low impedance resistor. Alternatively, a small aperture RF current transformer or a vacuum thermocouple may be used to measure the current flowing through the conductor between the two plates.

Instruments with a flat frequency response between 3 kHz and 100 MHz are available.

There are several issues that should be considered when selecting an instrument for measuring induced current.

Firstly, stand-on metres are subject to the influence of electric-field induced displacement currents from fields terminating on the top plate. Investigations have shown that apparent errors arising in the absence of a person are not material to the operation of the metres when a person is present.

Secondly, the sum of both ankle currents measured with clamp-on type metres tends to be slightly greater than the corresponding value indicated with plate type metres. The magnitude of this effect, which is a function the RF frequency and meter geometry, is not likely to be material. Nonetheless, the more accurate method of assessing limb currents is the current transformer. The precise method of measurement may depend upon the requirements of protection guidelines against which compliance assessments are made.

Thirdly, the ability to measure induced currents in limbs under realistic grounding conditions such as found in practice need to be considered. In particular, the differing degree of electrical contact between the ground and bottom plate of the parallel plate system and the actual ground surface may affect the apparent current flowing to ground.

Measurements can be made using antennas designed to be equivalent to a person. This enables a standardized approach to be used and permit current measurements to be made without the need for people to be exposed to potentially hazardous currents and fields.

3.2 Contact current measurement

The current measurement device has to be inserted between the hand of the person and the conductive object. The measurement technique may consist of a metallic probe (definite contact area) to be held by hand at one end of the probe while the other end is touched to the conductive object. A clamp-on current sensor (current transformer) can be used to measure the contact current which is flowing into the hand in contact with the conductive object.

Alternative methods are:

- the measurement of the potential difference (voltage drop) across a non-inductive resistor (resistance range of 5-10 Ω) connected in series between the object and the metallic probe holding in hand;
- a thermocouple milliammeter placed directly in series.

The wiring connections and the current meter must be set up in such way that interference and errors due to pick-up are minimized.

In the case where excessively high currents are expected an electrical network of resistors and capacitors can simulate the body's equivalent impedance.

3.3 Touch voltage measurement

The touch voltage (no-load-voltage) is measured by means of a suitable voltmeter or oscilloscope for the frequency range under consideration. The measurement devices are connected between the conductive object charged by field induced voltage and reference potential (ground). The input impedance of the voltmeter must not be smaller than 10 k Ω .

Appendix 5

Electromedical devices

1 Electromedical devices

Electromagnetic compatibility (EMC) is a general concern for electronic equipment and particularly electronic medical devices. EMF can affect electronic devices if the field strengths are high enough. Both the risk of EMC occurring and the level of it are dependent on distance between the radiating antenna and the device, the transmitter power, the frequency of the waves, the type of modulation of the radiated signal, the effect of cable coupling as well as the electronic devices own interference immunity.

RF interference to electromedical devices can usually be reduced or eliminated by suitable RF screening or electronic filtering. Applied techniques derived from those commonly used for EMC are suitable. Special limits, that may be significantly lower than general limits for population, may apply to medical devices, implanted or not, and to medical instrumentation.

1.1 Implanted and portable devices

EMF can cause RF interference to active implanted or portable medical devices.

Insulin pumps and cardiac pacemakers belong to this and, in the future, there may be an increasing number of these devices. Also the range and the number of different new devices appears to be increasing, e.g. portable monitors, prosthetic aids for sight and motion. Generally speaking, pacemakers and other medical devices could suffer interference from radiated EMF. However in the case of electromedical implanted devices, RF interference problems have not yet been completely solved due to the lack of full awareness of the problem for manufacturers and suppliers.

Appendix 6

References

- [1] IEC [6 October 2000] IEC Committee Draft (CD) 85/214/CD: Measurement and evaluation of high frequency (9 kHz to 300 GHz) electromagnetic fields with regard to human exposure.
 - [2] EBU [November 2001] BPN 023: Radio frequency radiation: Exposure limits and their implication for broadcasters. European Broadcasting Union
 - [3] ANSI/IEEE [1992] Standard for safety levels with respect to human exposure to radiofrequency electromagnetic fields, 3 kHz to 300 GHz. IEEE Std C95.1/D1.4.
 - [4] ICNIRP [April 1998] Guidelines for limiting exposure to time-varying electric, magnetic and electromagnetic fields (up to 300 GHz). *Health Physics*, Vol. 74, 4, p. 494-522.
 - [5] NRPB [1993] Board Statement on restrictions on human exposure to state and time varying electromagnetic fields and radiation. Doc. NRPB, Vol. 4, 5.
 - [6] CENELEC [21 November 2003] Draft prEN 50413: Basic Standard on measurement and calculation procedures for human exposure to electric, magnetic and electromagnetic fields (0 Hz-300 GHz).
 - [7] IEEE. IEEE Std C95.3: IEEE recommended practice for measurements and computations of radio frequency electromagnetic fields with respect to human exposure to such fields, 100 kHz-300 GHz.
-